

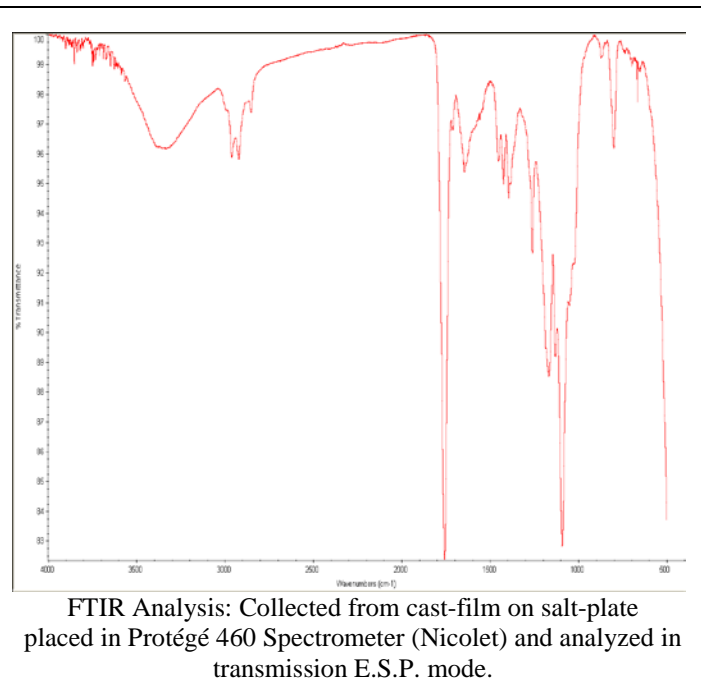


No. AI153 Certificate of Analysis

Product Name: Poly(lactide-co-glycolide) maleimide endcap (50:50 LA:GA, M_n : 25,000 – 35,000 Da) (Lot#: 70223JSG-E)

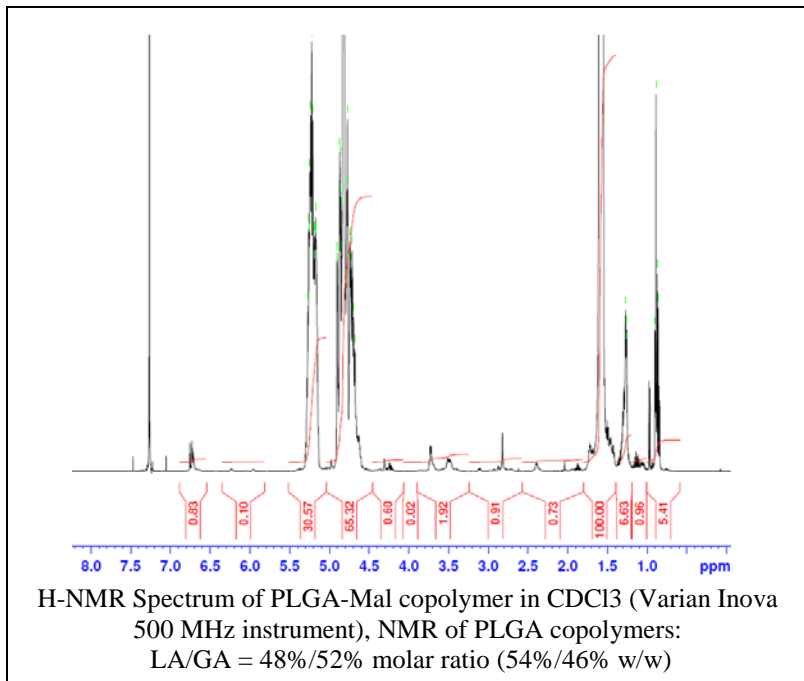

- **GPC analysis of PLGA copolymers**

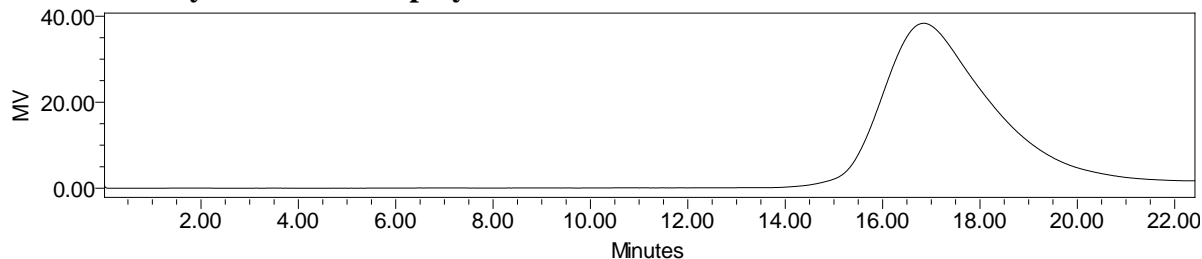

Analysis Method: Waters Breeze 2 system with 1 ml/min THF flow across three GPC columns (7.8 x 300 mm, mixed porosity). Detection via refractive index, calibrated against polystyrene standards.

Polymer	Mn (from GPC)	Mw (from GPC)	PDI
PLGA-Mal	28,696	49,058	1.71

- **Structure of PLGA-Maleimide copolymers**

