



# No. AP011 Certificate of Analysis

Product Name: Poly(caprolactone) copolymers free-acid endcap (Mn: 65,000- 75,000 Da)  
(Lot#: 50513FAJ)

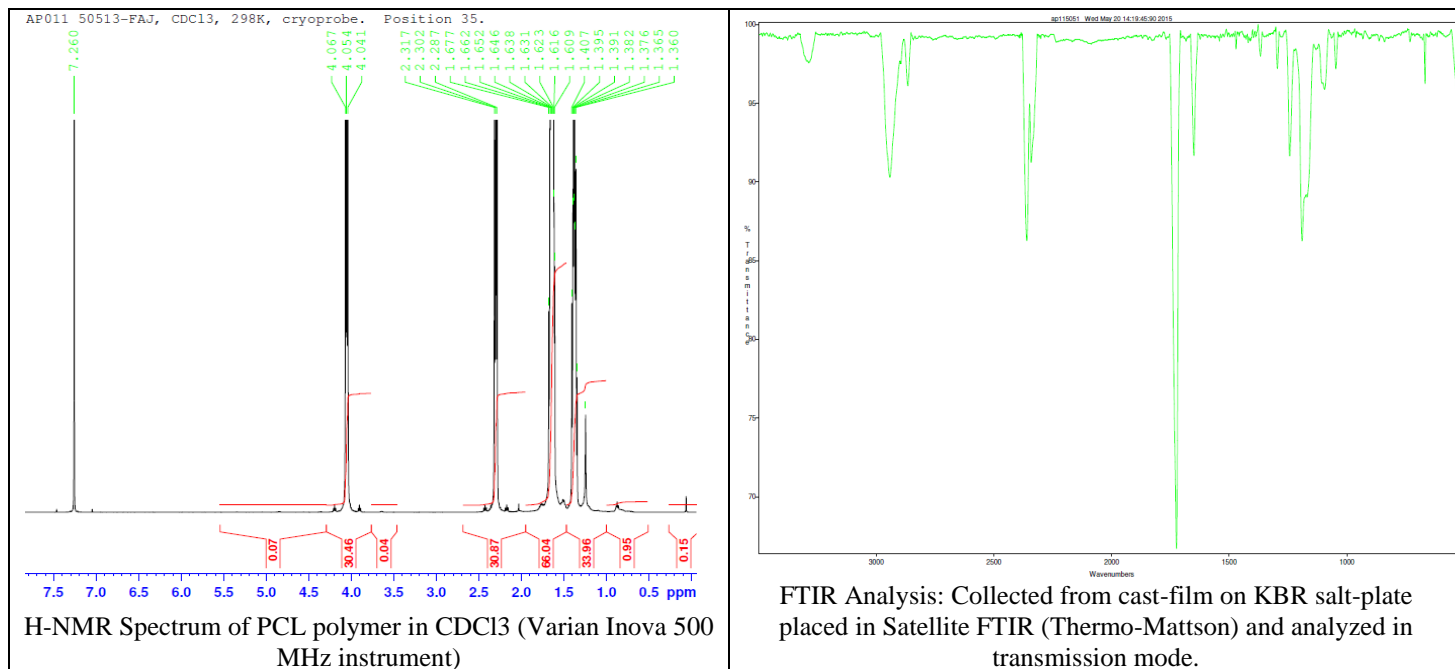


- GPC analysis of PCL copolymers

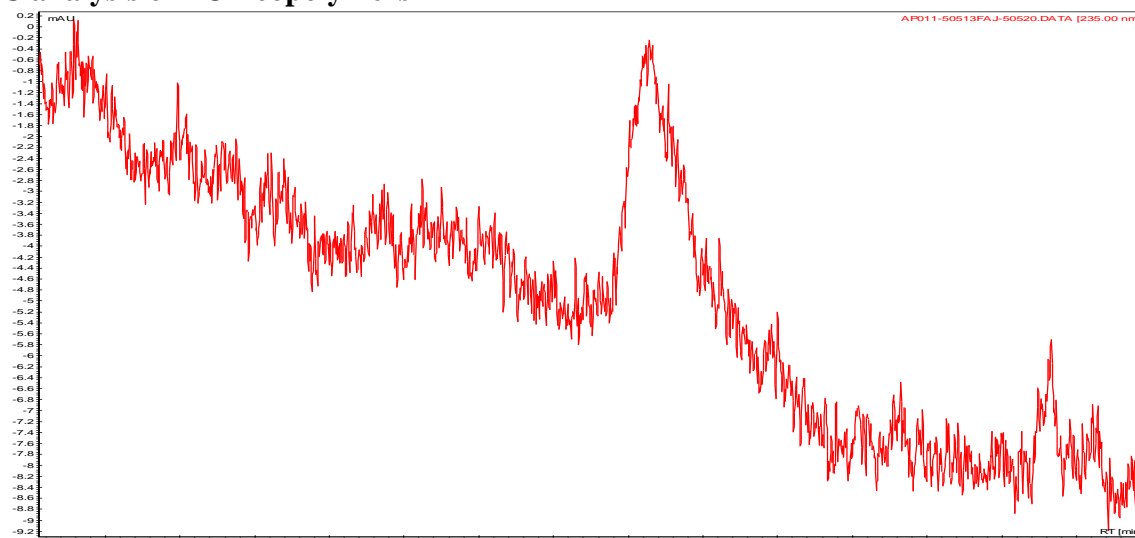

Analysis Method: Varian Prostar system with 1 ml/min DCM flow across two PLGel Resipore columns (Agilent). Detection via UV/Vis, calibrated against polystyrene standards.

Polymer	Mn (from GPC)	Mw (from GPC)	PDI
PCL	73,382	165,265	2.25

- Structure of PCL copolymers



Material provided for research use only. Not for human use.