



No. AP-34

Certificate of Analysis

Product Name: Poly(lactic-co-caprolactone) (1:99 LA:CL) ~75,000Da MW

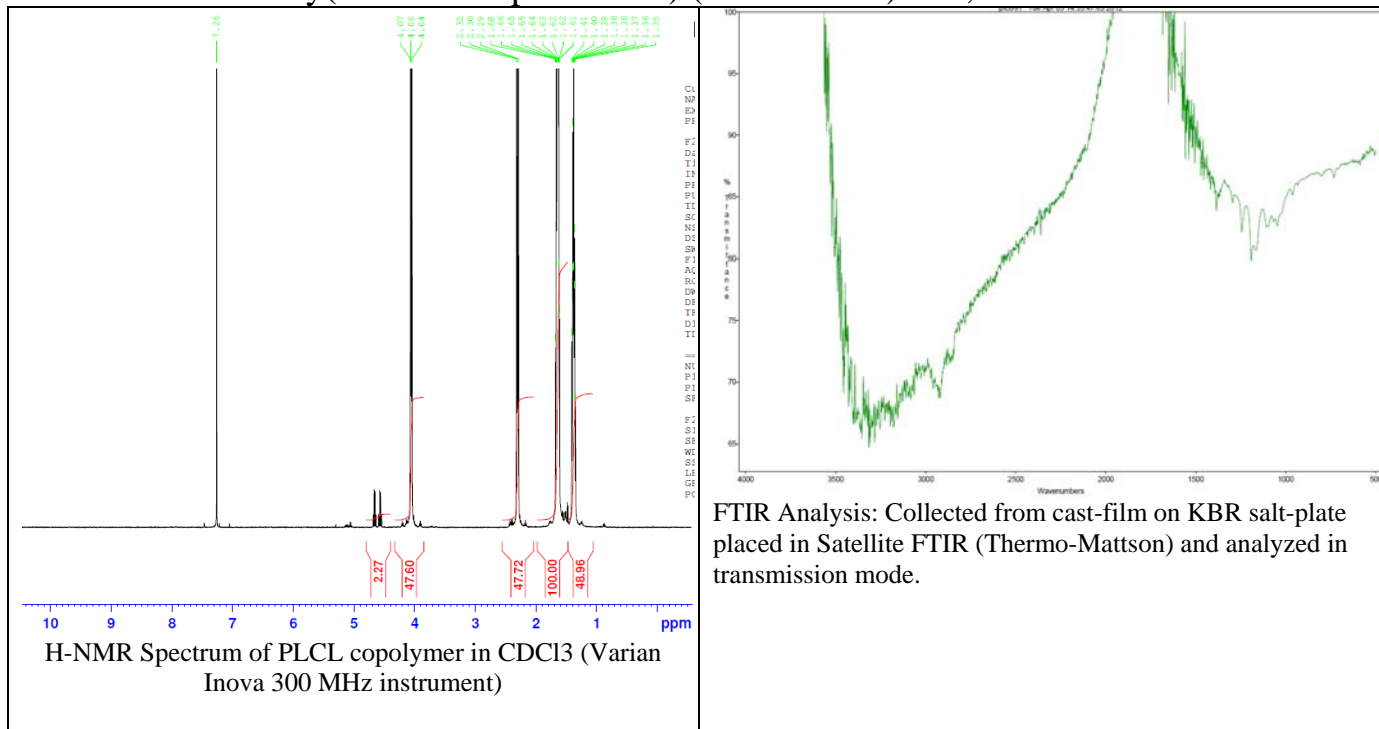

- GPC analysis of PLCL 99:1 copolymers

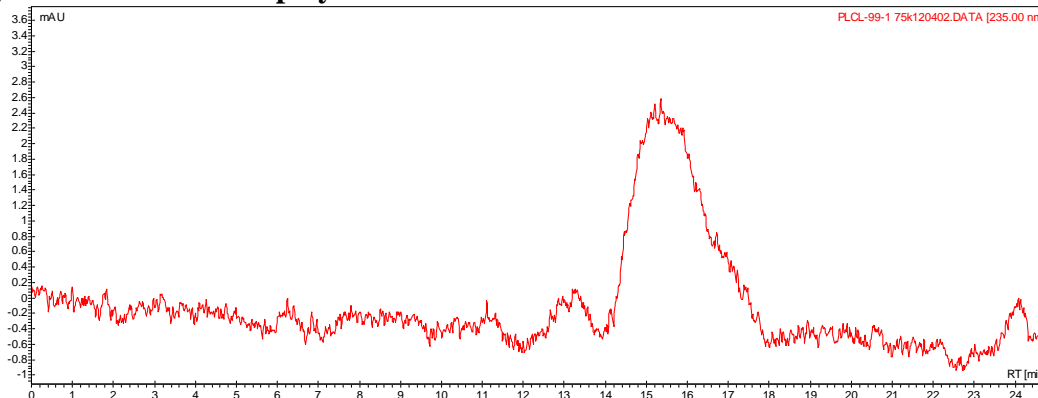

Analysis Method: Varian Prostar system with 1 ml/min DCM flow across two PLgel mixed-D columns and one Mixed-E column (Agilent). Detection via UV/Vis, calibrated against polystyrene standards

| Polymer | Mn (from GPC) | Mw (from GPC) | PDI |
|---------|---------------|---------------|------|
| AP34 | 59954 | 91715 | 1.53 |

- Structure of PLCL 99:1 copolymers

