
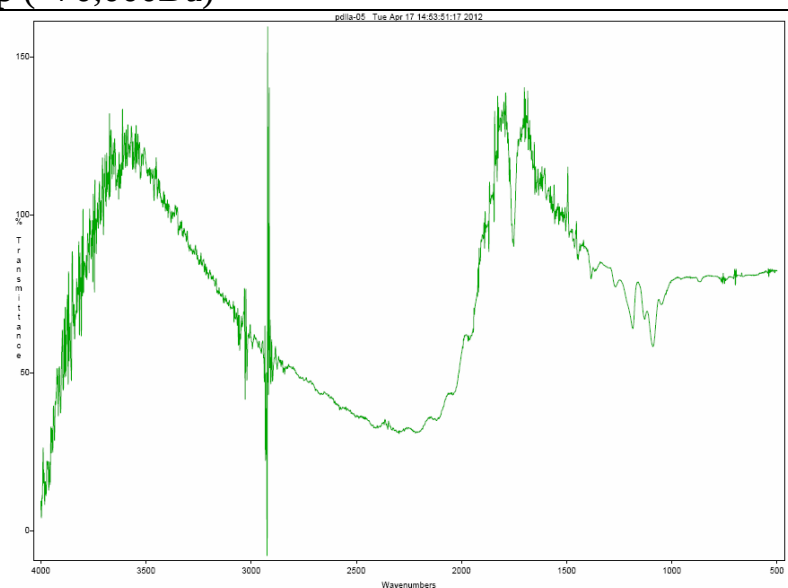



No. AP35

Certificate of Analysis

Product Name: Poly(D,L) Lactide Acid Endcap (~70,000Da)

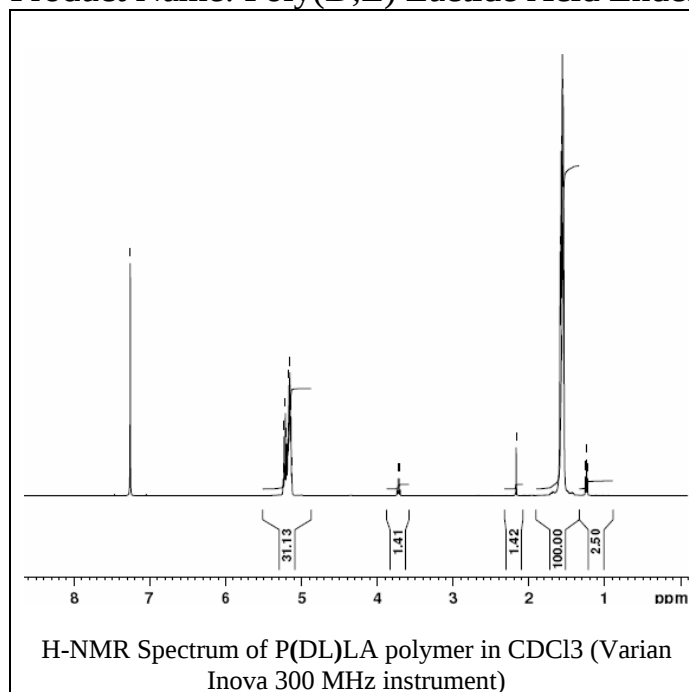

- GPC analysis of P(DL)LA polymer

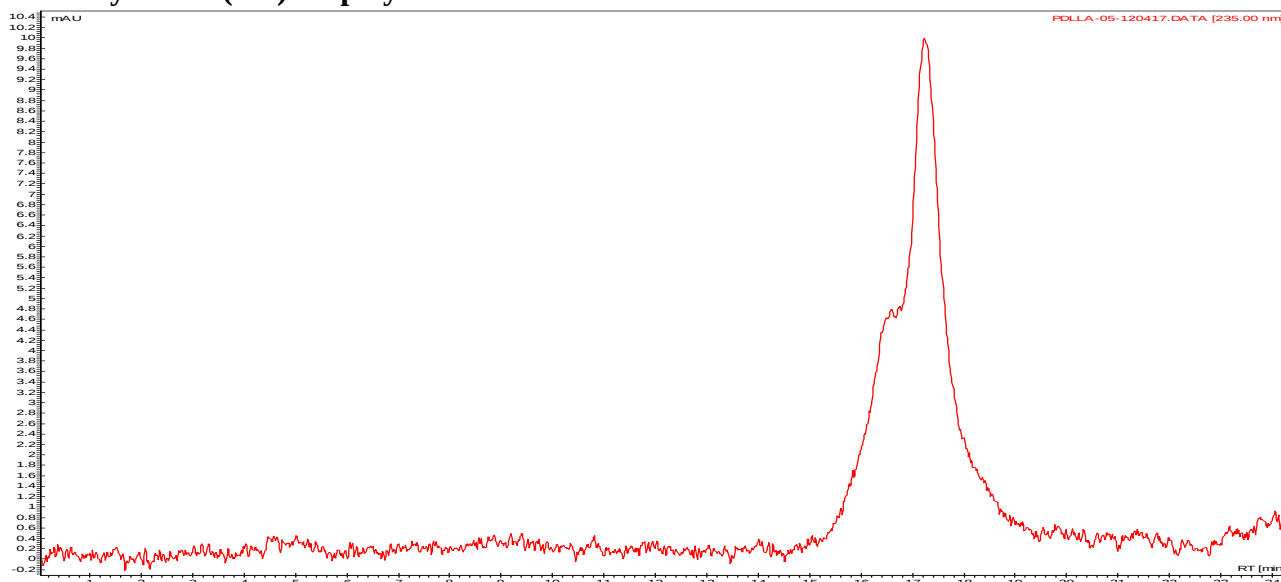

Analysis Method: Varian Prostar system with 1 ml/min DCM flow across two PLgel mixed-D columns and one Mixed-E column (Agilent). Detection via UV/Vis, calibrated against polystyrene standards

Polymer	Mn (from GPC)	Mw (from GPC)	PDI
P(DL)LA	56805	78058	1.37

- Structure of P(DL)LA polymer

