



# No. PLGA-60-35K Certificate of Analysis

Product Name: Poly(lactic-co-glycolic) copolymers

- <sup>1</sup>H-NMR Spectrum of PLGA copolymer in CDCl<sub>3</sub> (Varian Inova 300 MHz instrument)**

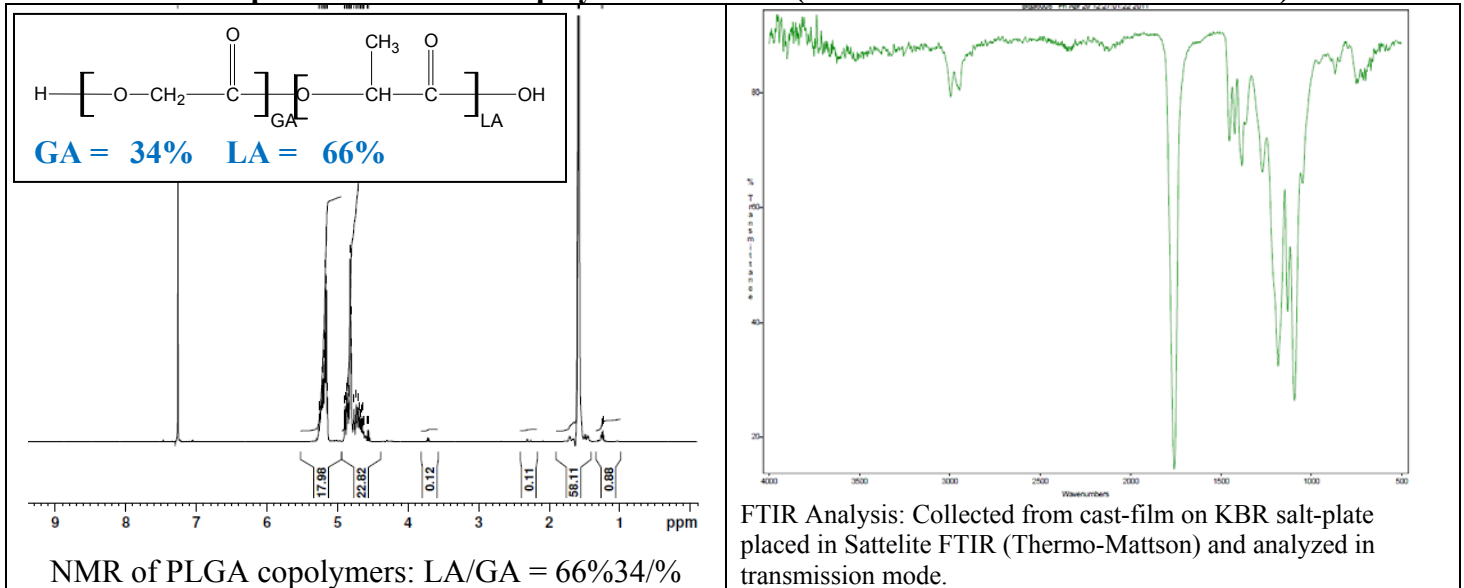

- GPC analysis of PLGA copolymers**

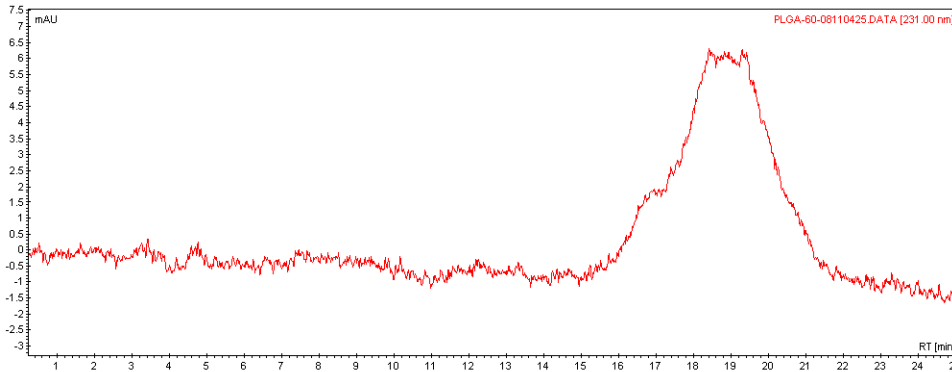

Analysis Method: Varian Prostar system with 1 ml/min DCM flow across two Resipore 3 um columns and one Mixed E column (Varian) and with UV-Vis (PDA) detection. Calibrated against polystyrene standards

Polymer	Mn (from GPC)	Mw (from GPC)	PDI
PLGA60-35k (PLGA-60-08)	31982	37644	1.18

- Inherent Viscosity 0.73 dl/g (measured at 25°C in chloroform)**