



No. AI010

Certificate of Analysis

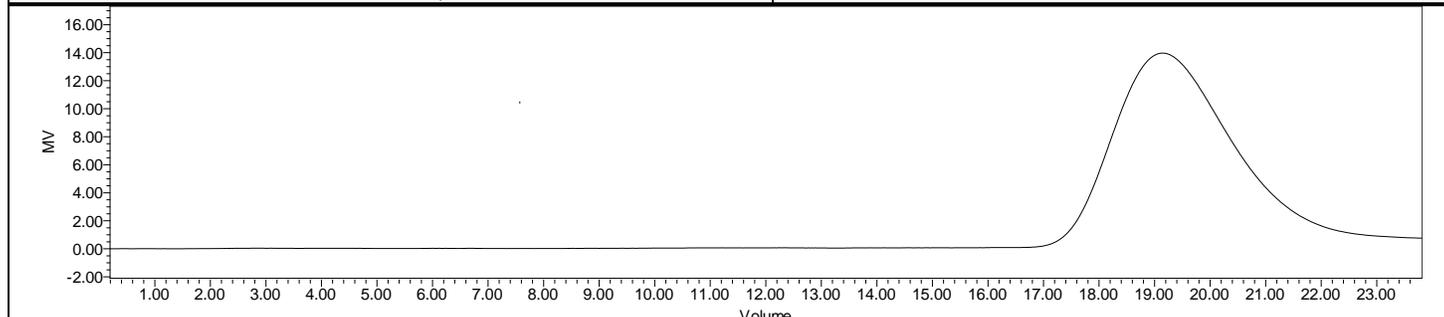

Product Name: Poly(lactide-co-glycolide) amine endcap
(Mn: 15,000-35,000 Da) (Lot#: 190520RAI-B)

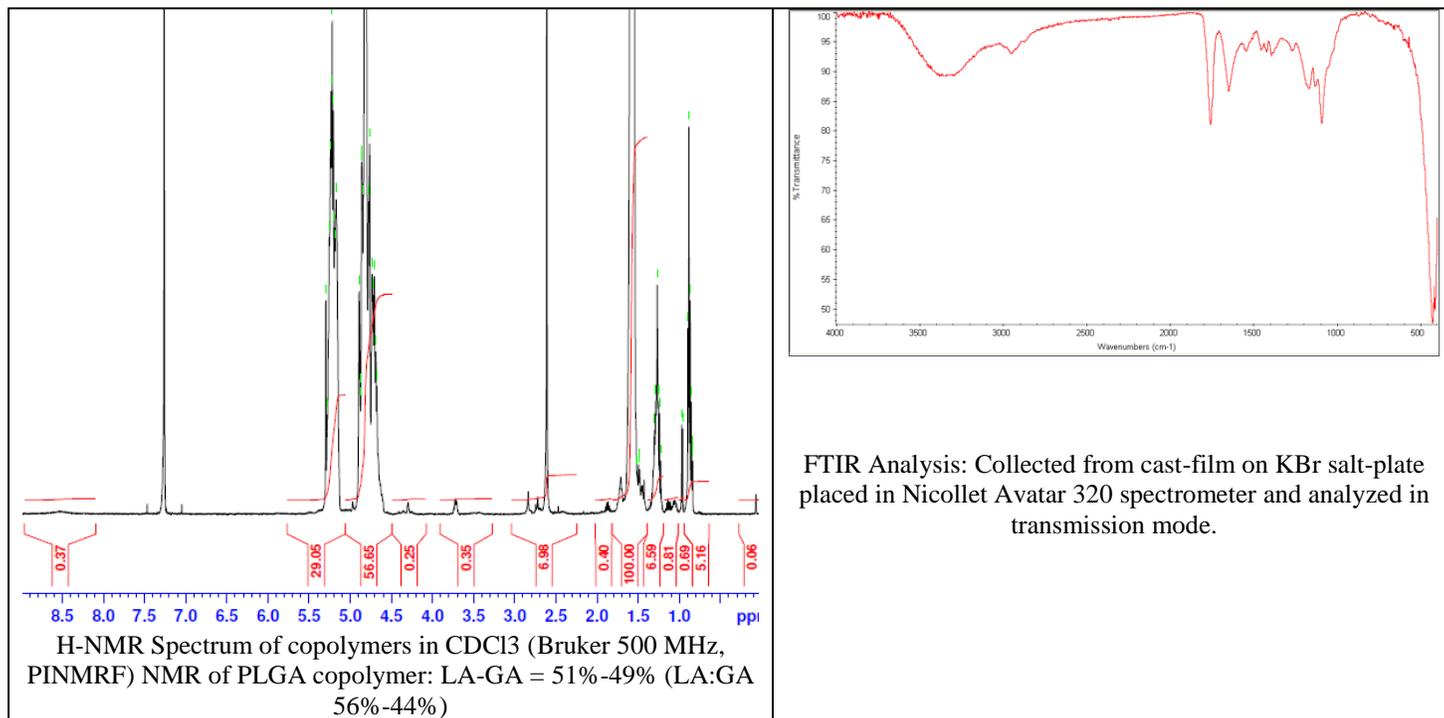

GPC Analysis Method: Waters Breeze 2 system with 1 ml/min THF flow across three GPC columns. Detection via refractive index, calibrated against polystyrene standards.

Polymer	M _n (from GPC)	M _w (from GPC)	PDI
PLGA	32,219	44,676	1.39

• Structure of PLGA-NH₂ copolymers

