



FTIR

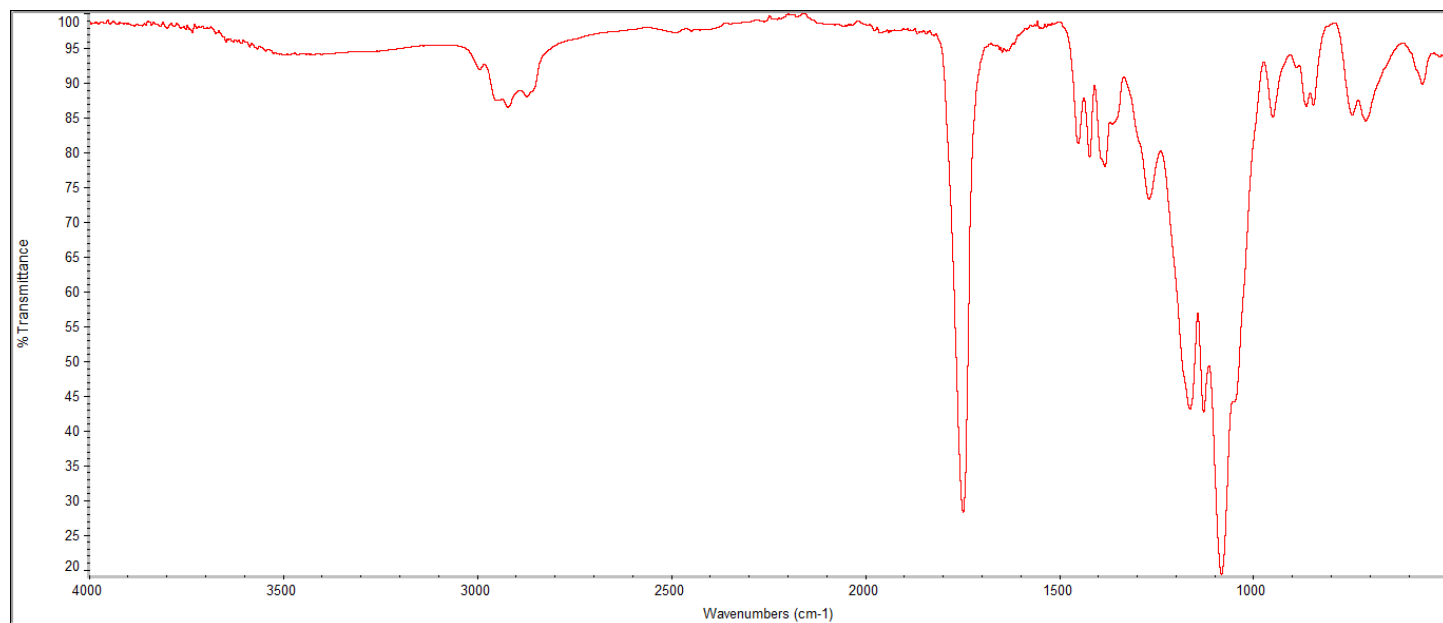

FTIR Analysis: Collected from IS5 ID7-ATR spectrometer (Thermo Scientific) and analyzed in transmission mode.

GPC-ES

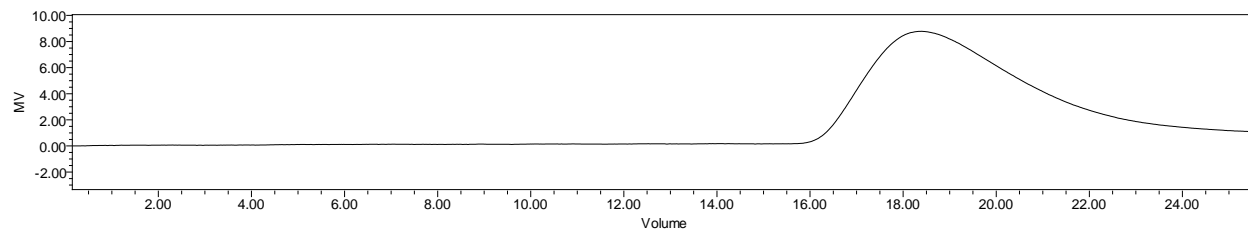

Polymer	M _n (from GPC)	M _w (from GPC)	PDI
PLGA-PEG-COOH	18,413	37,304	2.03
PEG-precursor*	4500*		

GPC-ES Analysis Method: Waters Breeze 2 system with 1 ml/min THF flow across three GPC columns. Detection via refractive index, calibrated against polystyrene standards. *from MFG data


DSC

Sample: AI078 260608RAI-A
Size: 4.8000 mg
Method: Ramp

DSC

File: C:\...\COA\AI078 260608RAI-A.001

Run Date: 12-Jun-2026 12:12
Instrument: DSC Q2000 V24.11 Build 124

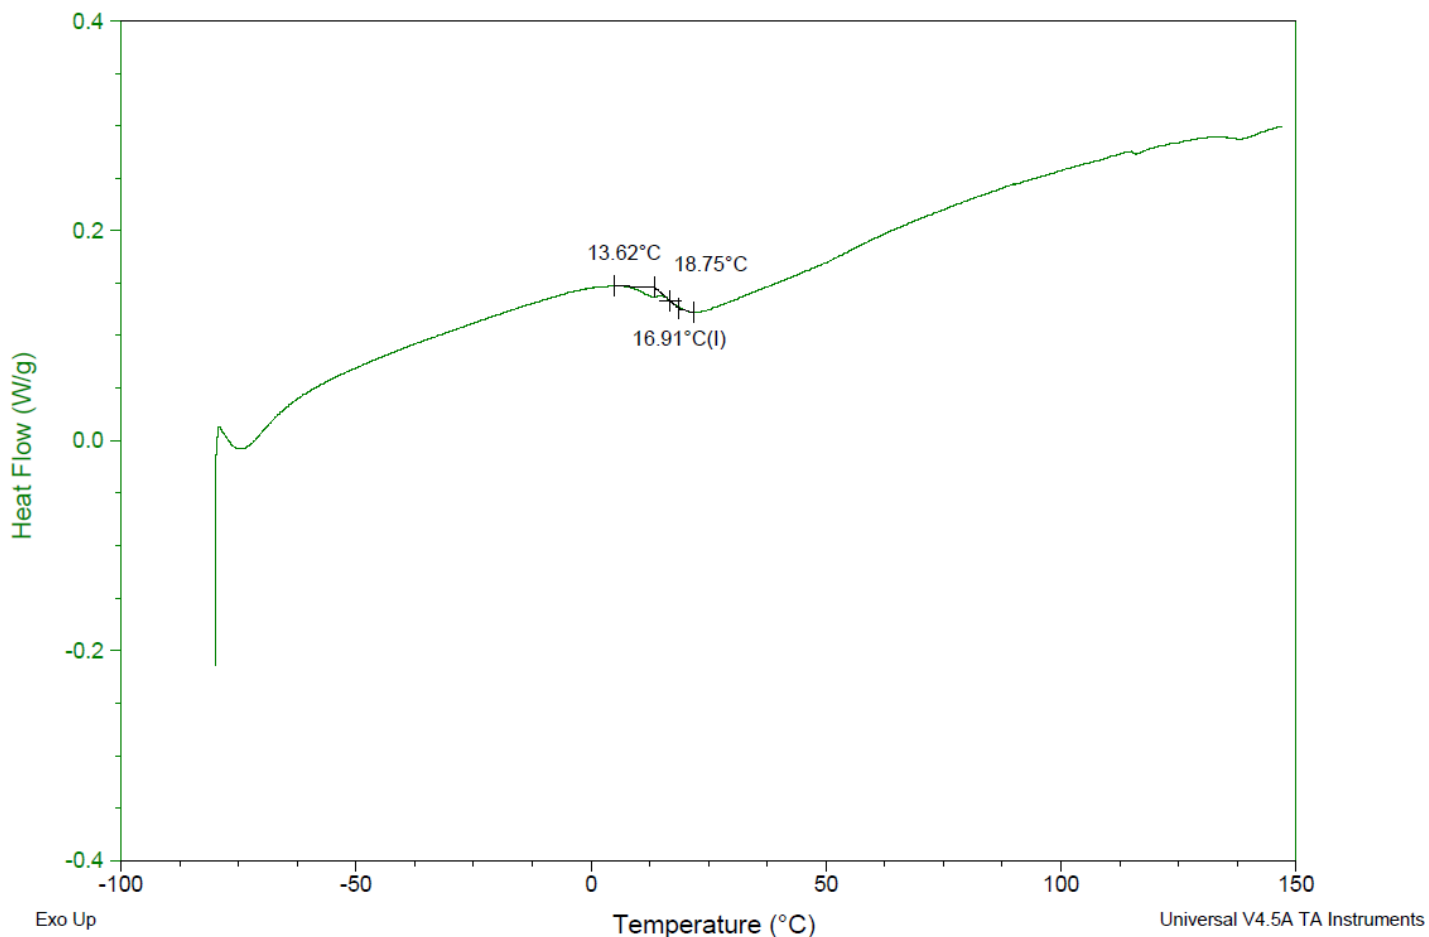


DSC Testing: 1-5 mg sample tested in crimped aluminum pan on a TA Instruments Model Q2000 with procedure equilibraion 100 °C, isothermal 5 minutes, equilibrate -80 °C, data on, ramp 10 °C/min to 150 °C. Tg = 18.75 °C

IV

Inherent Viscosity: 0.282 ± 0.017 dL/g (calculated from kinematic viscosity at 2% w/v Acetone on Rheosense microVISC, n=3) at 25°C.

Structure of copolymers

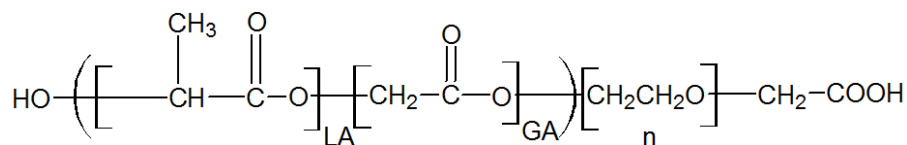

Approved By:
Amie Tyler
Quality Manager