



FTIR

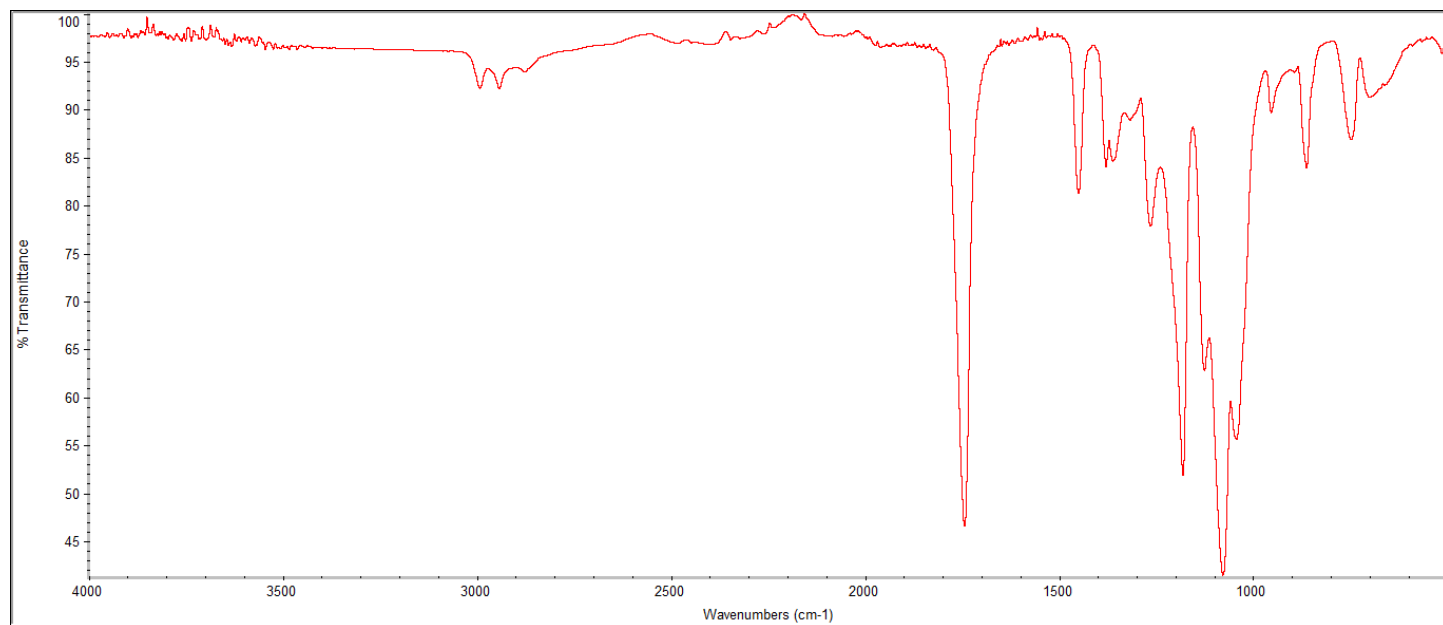

FTIR Analysis: Collected from IS5 ID7-ATR spectrometer (Thermo Scientific) and analyzed in transmission mode.

GPC-ES

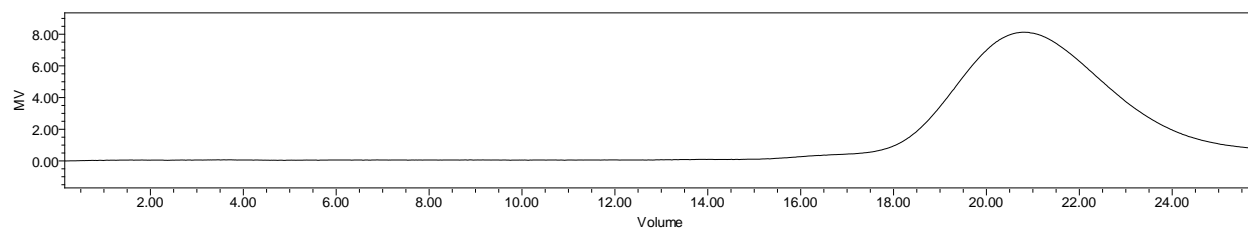

Polymer	M _n (from GPC)	M _w (from GPC)	PDI
PDLLA-PEG-PDLLA	13,144	17,586	1.34
PEG-Precursor*	1013*		

GPC-ES Analysis Method: Waters Breeze 2 system with 1 ml/min THF flow across three GPC columns. Detection via refractive index, calibrated against polystyrene standards. *- from MFG data

DSC


Sample: AK059 260527TMT-A
Size: 4.5000 mg
Method: Ramp

DSC

File: C:\...COA\AK059 260527TMT-A.001

Run Date: 04-Jun-2026 09:44

Instrument: DSC Q2000 V24.11 Build 124

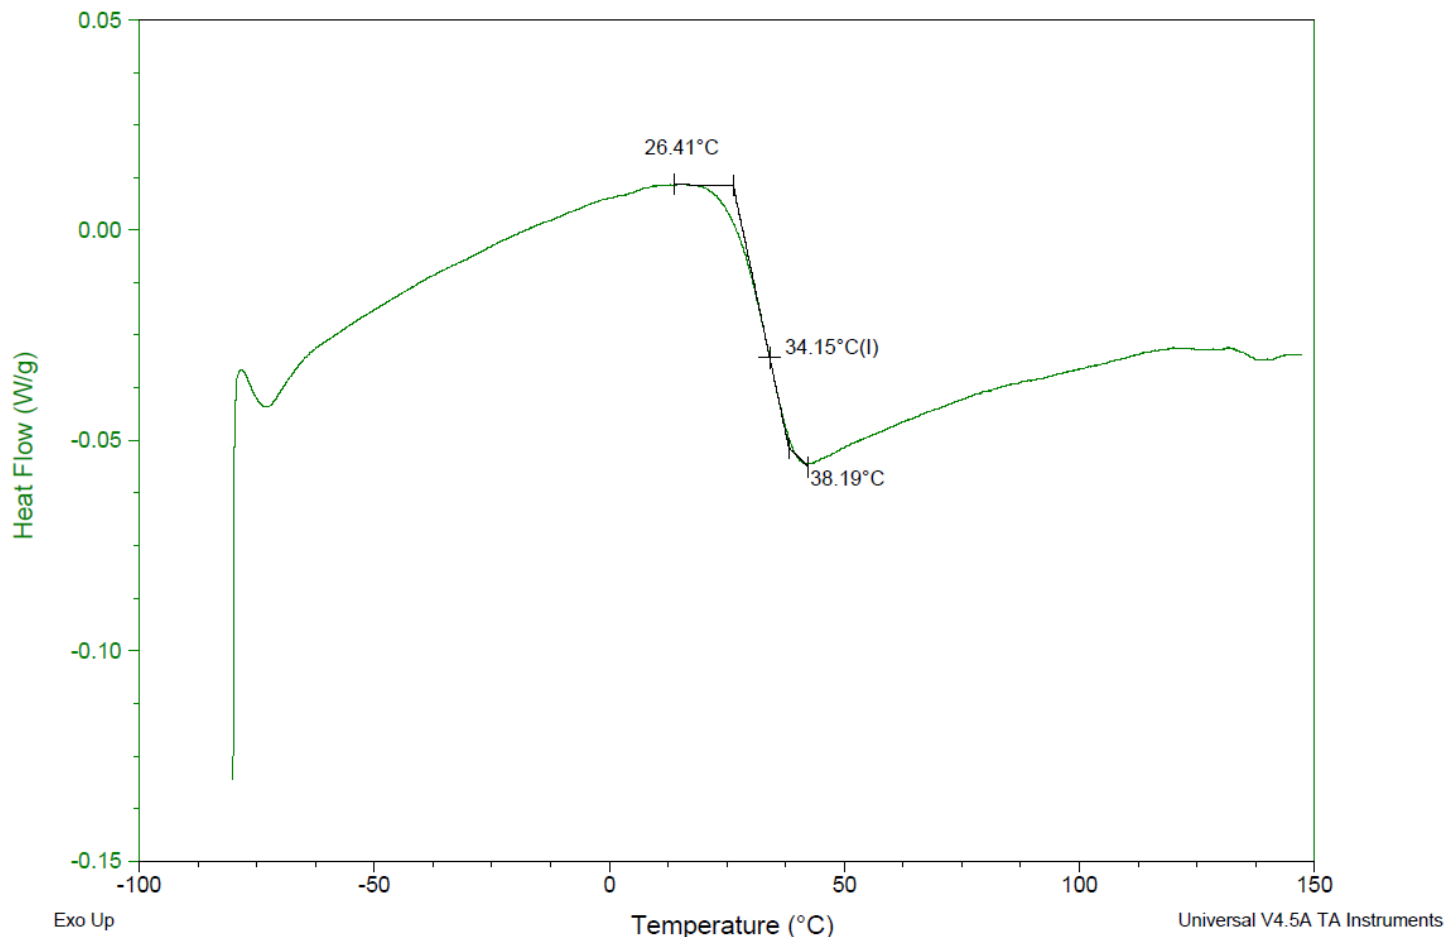


DSC Testing: 1-5 mg sample tested in crimped aluminum pan on a TA Instruments Model Q2000 with procedure equilibraion 100 °C, isothermal 5 minutes, equilibrate -80 °C, data on, ramp 10 °C/min to 150 °C. Tg = 34.15 °C

IV

Inherent Viscosity: 0.203 ± 0.029 dL/g (calculated from kinematic viscosity at 2% w/v Acetone on Rheosense microVISC, n=3) at 25°C.

Structure of copolymers

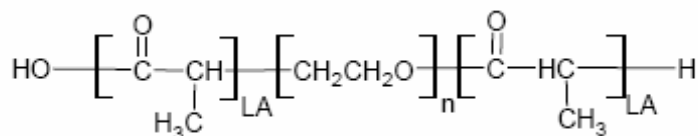

Approved By:
Amie Tyler
Quality Manager