


No. AP015

Certificate of Analysis




Product Name: Poly(L-lactide-co-caprolactone) copolymer acid endcap (50:50 LA:CL,
 M_n : 75,000-85,000 Da) (Lot#: 250611DJR-A)

H-NMR

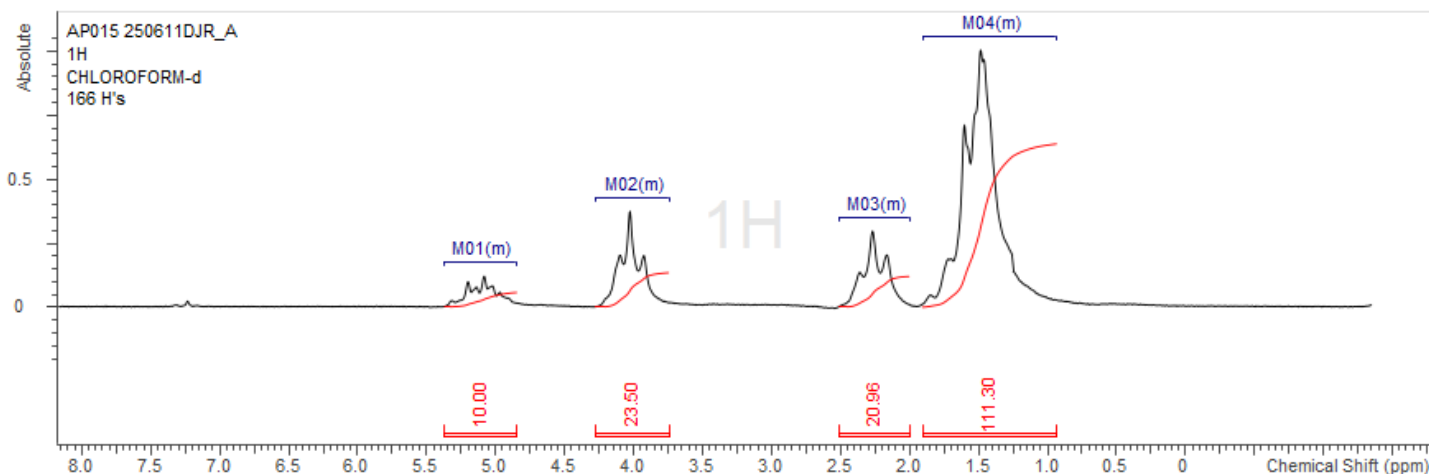


H-NMR Spectrum of copolymers in $CDCl_3$ (NMReady-60e, Nanalysis 60 MHz) NMR of PLLCL copolymer: LA-CL =46%-54% molar ratio (LA:CL 35%:65% w:w)

FTIR

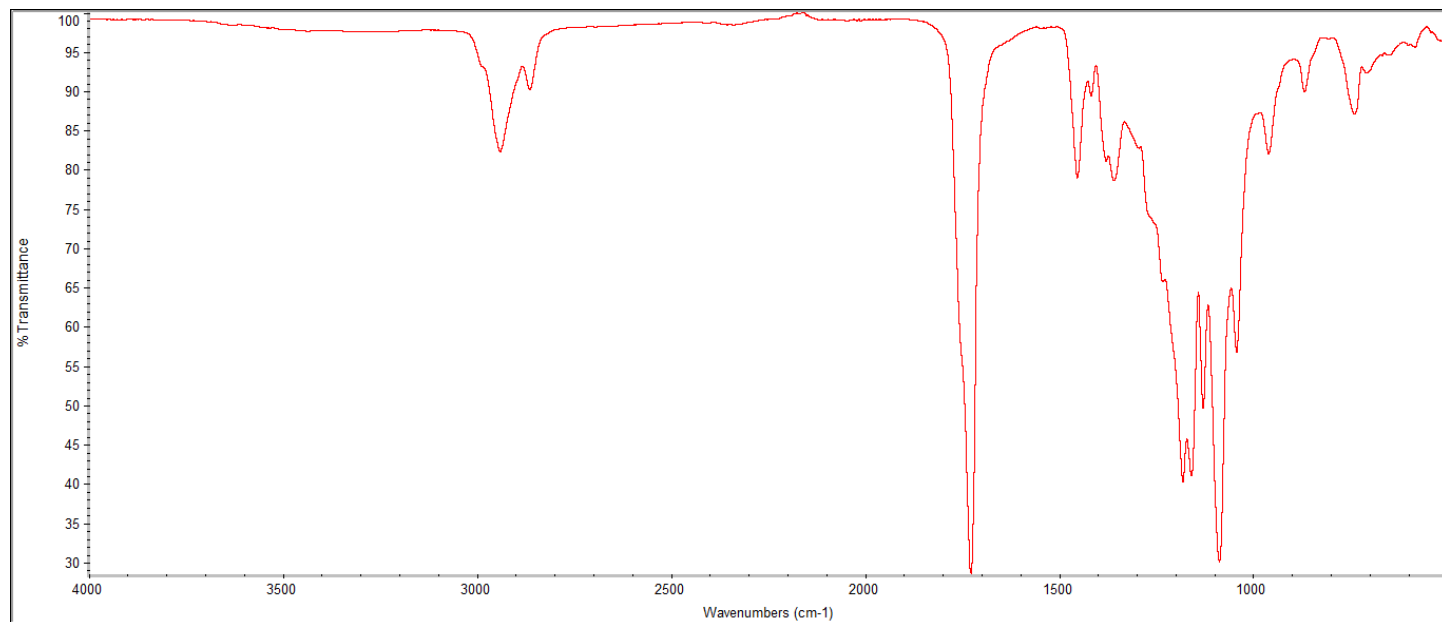

FTIR Analysis: Collected from IS5 ID7-ATR spectrometer (Thermo Scientific) and analyzed in transmission mode.

GPC-ES

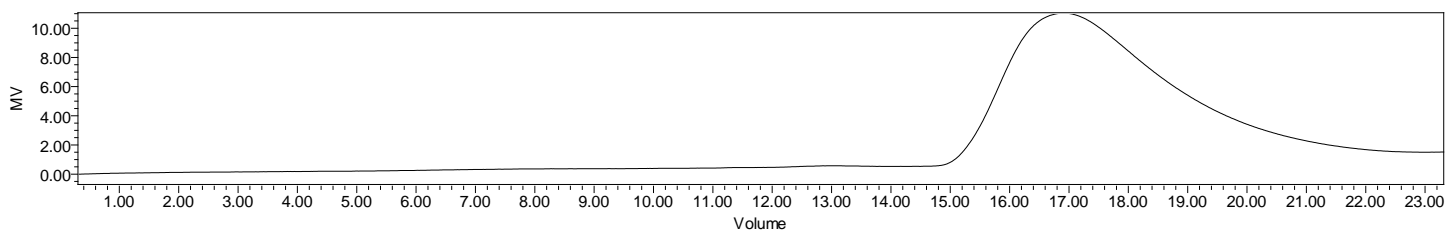

Polymer	M _n (from GPC)	M _w (from GPC)	PDI
PLLCL	76,324	98,281	1.29

GPC-ES Analysis Method: Waters Breeze 2 system with 1 ml/min THF flow across three GPC columns. Detection via refractive index, calibrated against polystyrene standards.

DSC


Sample: AP160 250611DJR-A
Size: 4.7000 mg
Method: Ramp

DSC

File: C:\...\COA\AP160 250611DJR-A DSC.002

Run Date: 18-Jun-2025 08:31

Instrument: DSC Q2000 V24.11 Build 124

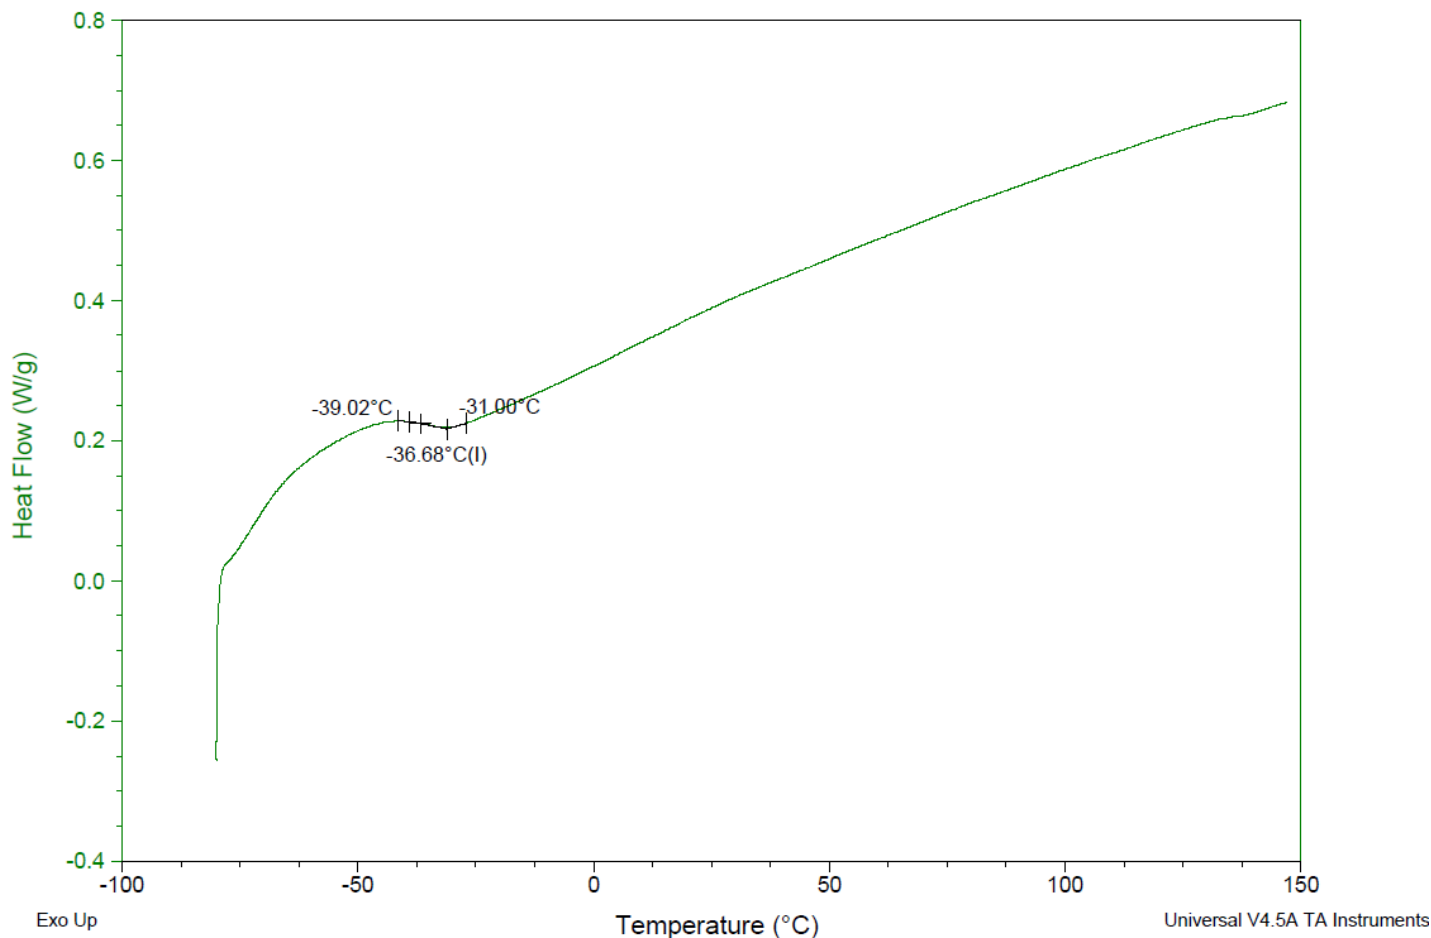


DSC Testing: 1-5 mg sample tested in crimped aluminum pan on a TA Instruments Model Q2000 with procedure equilibraion 100 °C, isothermal 5 minutes, equilibrate -80 °C, data on, ramp 10 °C/min to 150 °C. T_g = -36.68 °C

IV

Inherent Viscosity: 0.529 ± 0.171 dL/g (calculated from kinematic viscosity at 2% w/v Acetone on Rheosense microVISC, n=3) at 25°C.

Structure of copolymers

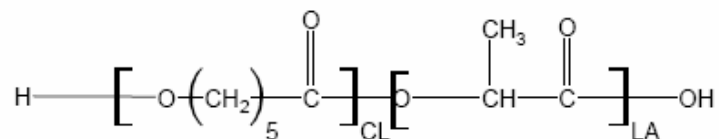

Approved By:
Amie Tyler
Quality Manager