



No. AP-34
Certificate of Analysis

Product Name: Poly(lactic-co-caprolactone) (1:99 LA:CL) ~75,000Da MW

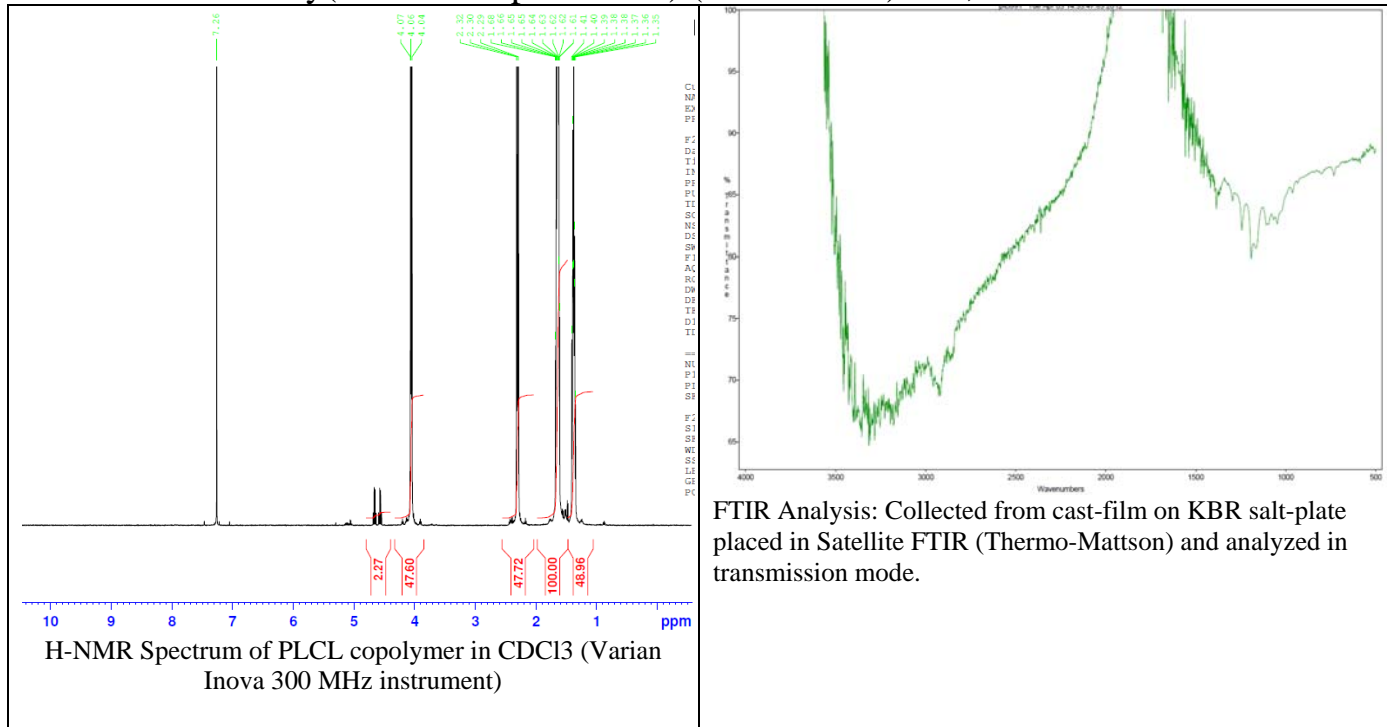

- GPC analysis of PLCL 99:1 copolymers**

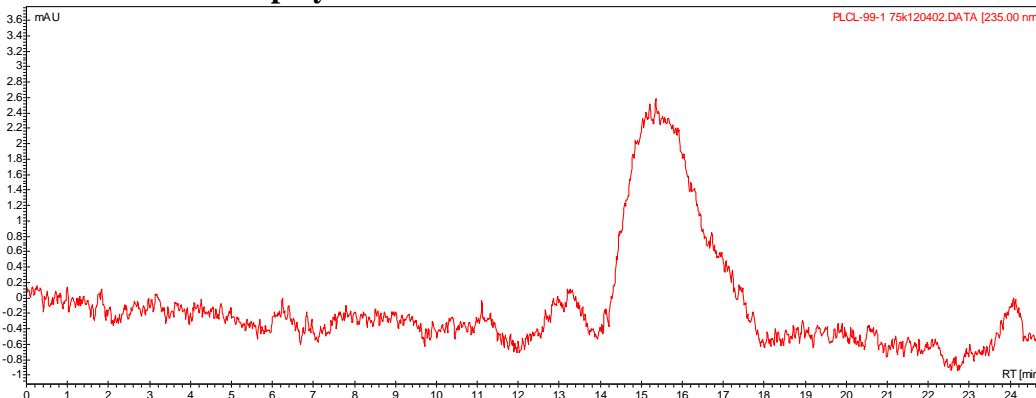

Analysis Method: Varian Prostar system with 1 ml/min DCM flow across two PLgel mixed-D columns and one Mixed-E column (Agilent). Detection via UV/Vis, calibrated against polystyrene standards

Polymer	Mn (from GPC)	Mw (from GPC)	PDI
AP34	59954	91715	1.53

- Structure of PLCL 99:1 copolymers**

