


**No. AP067**

# Certificate of Analysis




Product Name: Poly(L-Lactic-co-caprolactone) Copolymer ester endcap (50:50 LA:CL,  
 $M_n$ : 45,000-55,000 Da) (Lot#: 250516DJR-A)

## H-NMR

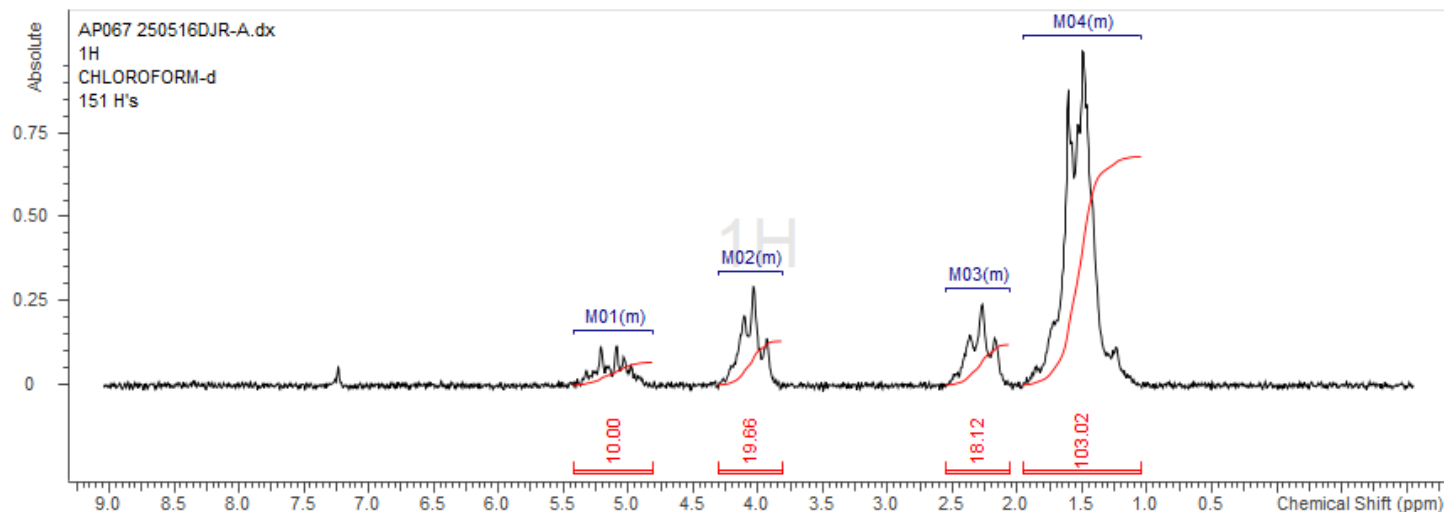


**H-NMR** Spectrum of copolymers in  $CDCl_3$  (NMReady-60e, Nanalysis 60 MHz) NMR of PLCL copolymer: LA-CL =50%-50% molar ratio (LA:GA 56%:44% w:w)

## FTIR

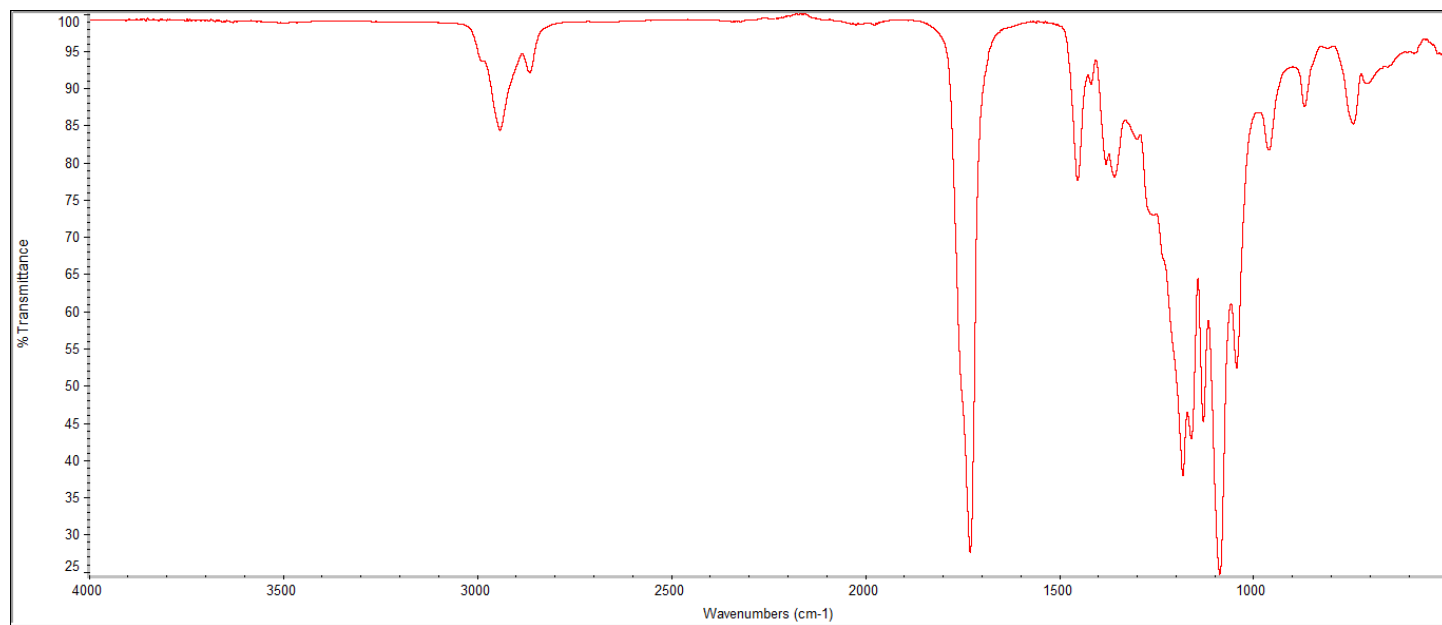

**FTIR** Analysis: Collected from IS5 ID7-ATR spectrometer (Thermo Scientific) and analyzed in transmission mode.

## GPC-ES

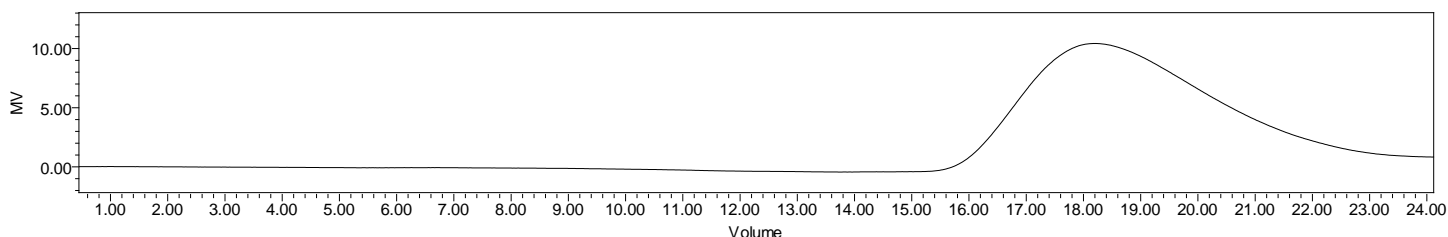

Polymer	M <sub>n</sub> (from GPC)	M <sub>w</sub> (from GPC)	PDI
PLGA	45,436	54,535	1.20

**GPC-ES Analysis Method:** Waters Breeze 2 system with 1 ml/min THF flow across three GPC columns. Detection via refractive index, calibrated against polystyrene standards.


## DSC

Sample: AP067 250516DJR-A  
Size: 4.1000 mg  
Method: Ramp

### DSC

File: C:\...\COA\AP067 250516DJR-A.002

Run Date: 23-May-2025 08:29  
Instrument: DSC Q2000 V24.11 Build 124

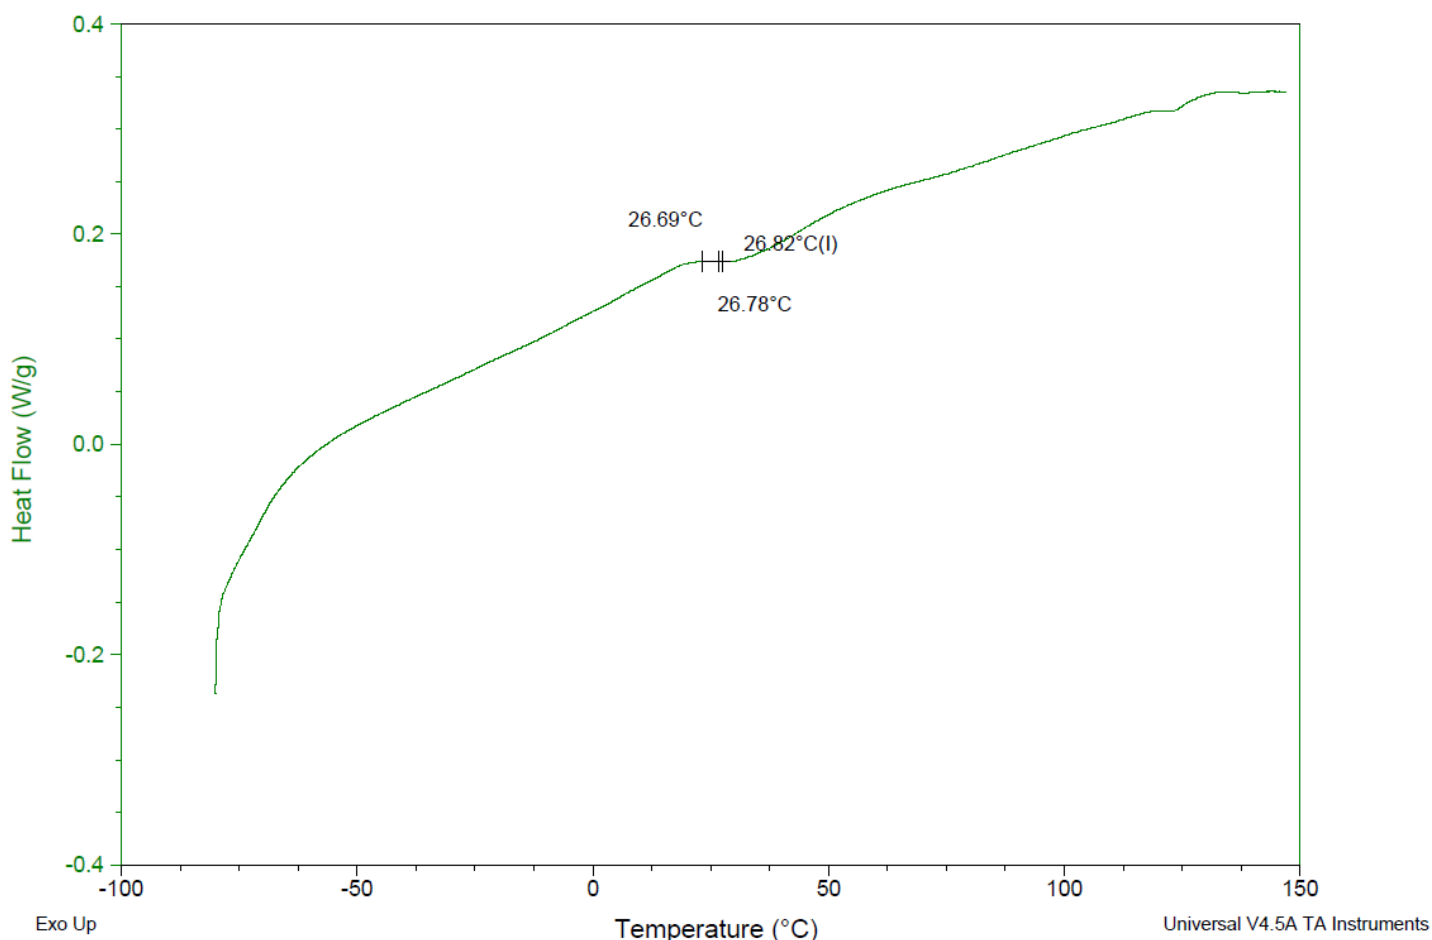


**DSC Testing:** 1-5 mg sample tested in crimped aluminum pan on a TA Instruments Model Q2000 with procedure equilibraion 100 °C, isothermal 5 minutes, equilibrate -80 °C, data on, ramp 10 °C/min to 150 °C. T<sub>g</sub> = 26.82 °C

## IV

**Inherent Viscosity:**  $0.257 \pm 0.001$  dL/g (calculated from kinematic viscosity at 2% w/v Acetone on Rheosense microVISC, n=3) at 25°C.

### Structure of copolymers

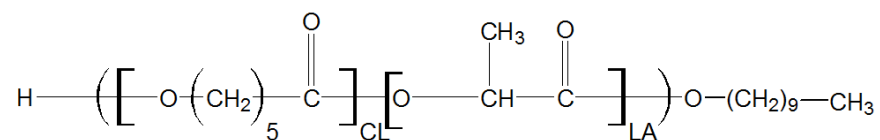

Approved By:  
*Amie Tyler*  
Quality Manager