


No. AP081

# Certificate of Analysis




Product Name: Poly(lactide-co-glycolide) acid endcap (50:50 LA:GA) (Mn: 5,000-10,000 Da)  
(Lot#: 260422RAI-A)

## H-NMR

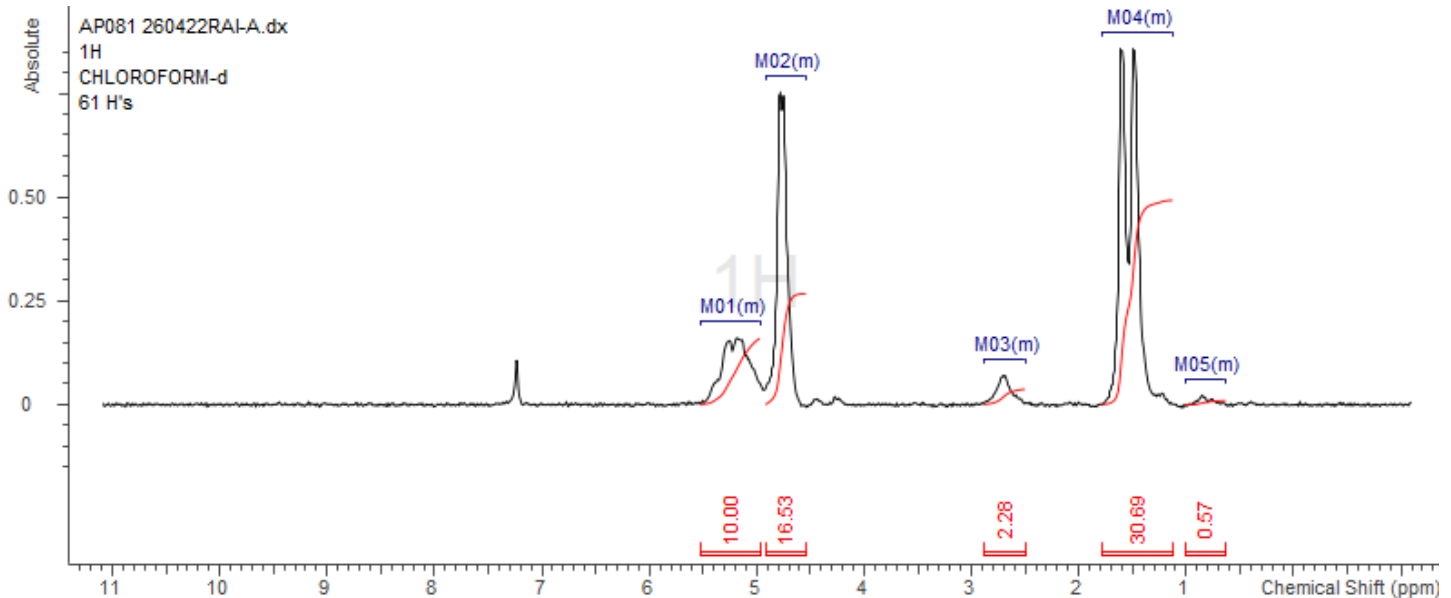


H-NMR Spectrum of copolymers in CDCl<sub>3</sub> (NMReady-60e, Nanalysis 60 MHz) NMR of PLGA copolymer: LA-GA =55%-45% molar ratio (LA:GA 60%:40% w:w)

## FTIR

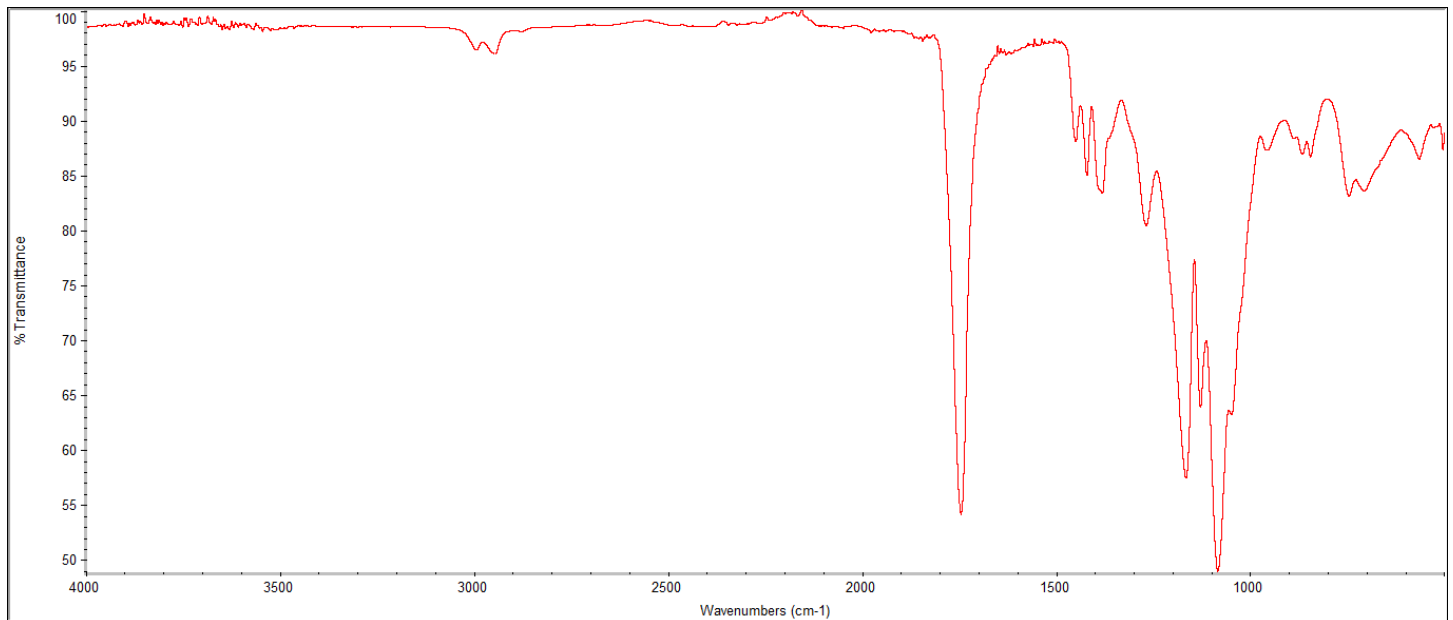

FTIR Analysis: Collected from IS5 ID7-ATR spectrometer (Thermo Scientific) and analyzed in transmission mode.

## GPC-ES

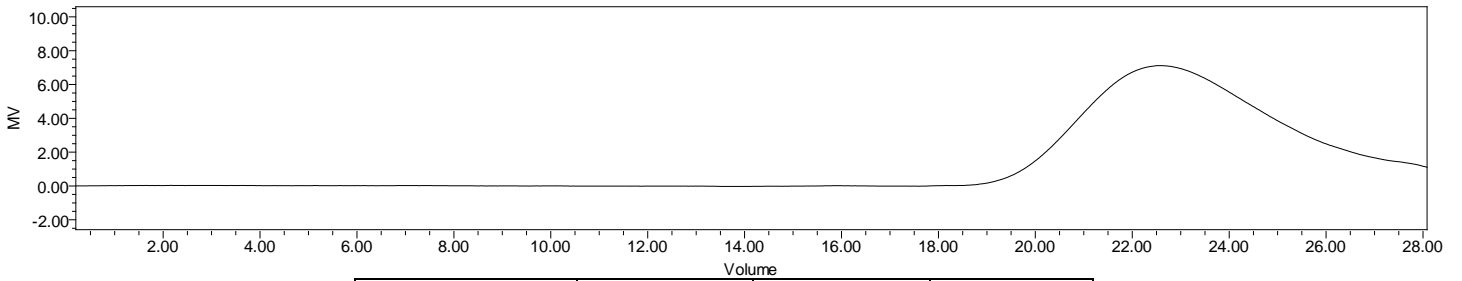

| Polymer | M <sub>n</sub> (from GPC) | M <sub>w</sub> (from GPC) | PDI  |
|---------|---------------------------|---------------------------|------|
| PLGA    | 6422                      | 9059                      | 1.41 |

**GPC-ES Analysis Method:** Waters Breeze 2 system with 1 ml/min THF flow across three GPC columns. Detection via refractive index, calibrated against polystyrene standards.


## DSC

Sample: AP081 260422RAI-A  
 Size: 4.5000 mg  
 Method: Ramp

### DSC

File: C:\...\COA\AP081 260422RAI-A.001

Run Date: 28-Apr-2026 10:03  
 Instrument: DSC Q2000 V24.11 Build 124

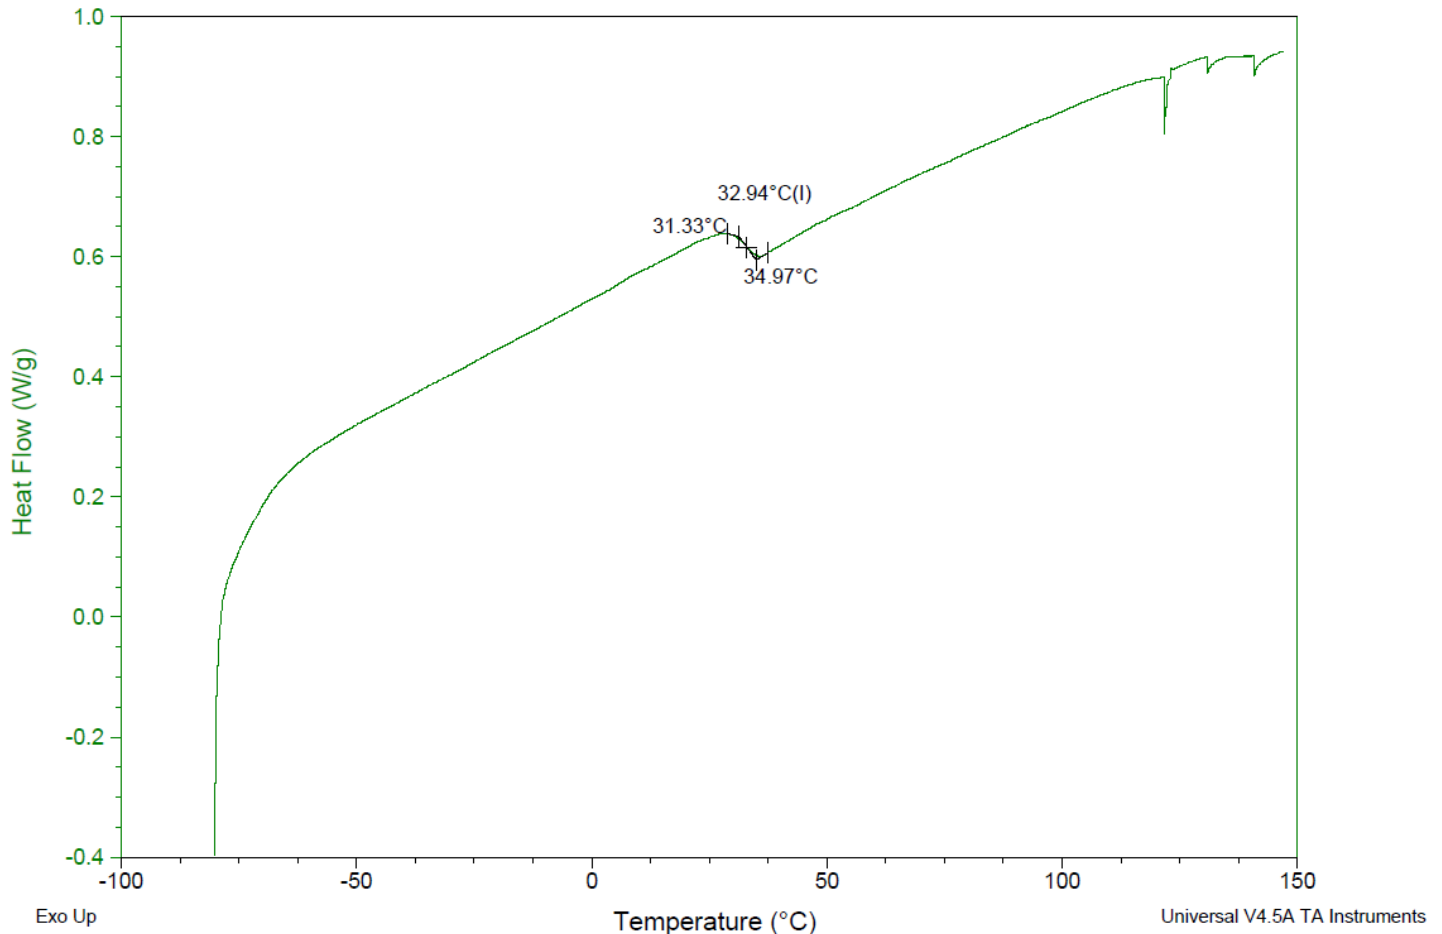


**DSC Testing:** 1-5 mg sample tested in crimped aluminum pan on a TA Instruments Model Q2000 with procedure equilibraion 100 °C, isothermal 5 minutes, equilibrate -80 °C, data on, ramp 10 °C/min to 150 °C. T<sub>g</sub> = 32.94 °C

## IV

**Inherent Viscosity:**  $0.120 \pm 0.020$  dL/g (calculated from kinematic viscosity at 2% w/v Acetone on Rheosense microVISC, n=3) at 25°C.

### Structure of copolymers

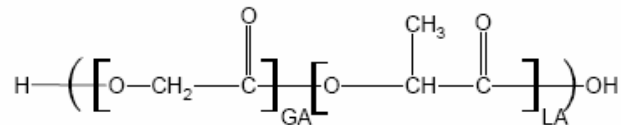

Approved By:  
*Amie Tyler*  
Quality Manager