


No. AP324

Certificate of Analysis




Product Name: Poly(L-Lactic-co-caprolactone) copolymer ester endcap (40:60 LA:CL,
Mn: 55,000-65,000 Da) (Lot#: 250728DJR-A)

H-NMR

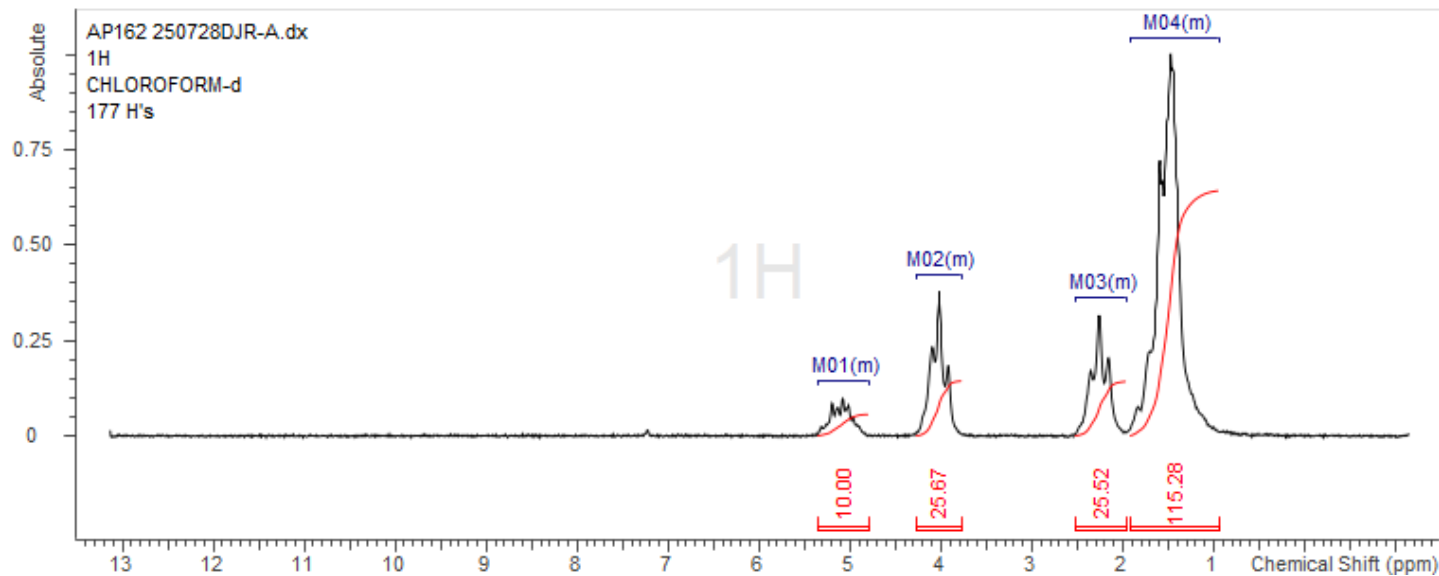


H-NMR Spectrum of copolymers in CDCl₃ (NMReady-60e, Nanalysis 60 MHz) NMR of P(L)LCL copolymer: LA-CL =44%-56% molar ratio (LA:CL 33%:67% w:w)

FTIR

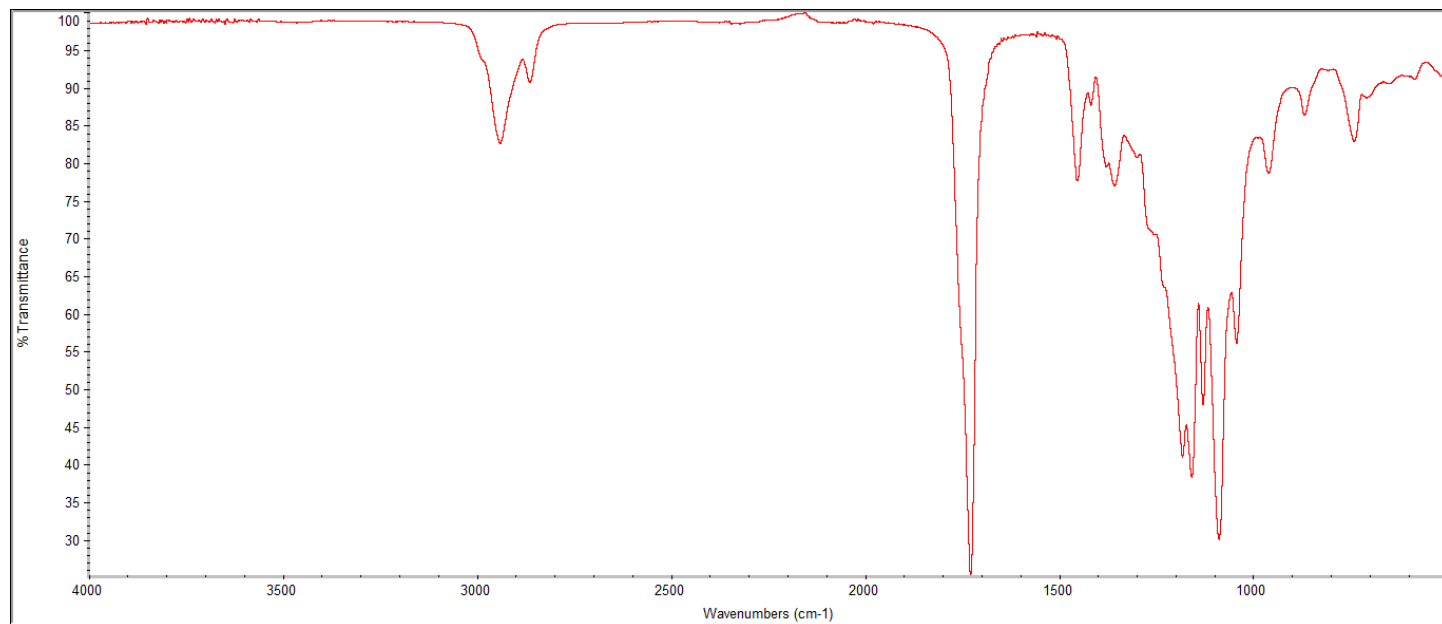

FTIR Analysis: Collected from IS5 ID7-ATR spectrometer (Thermo Scientific) and analyzed in transmission mode.

GPC-ES

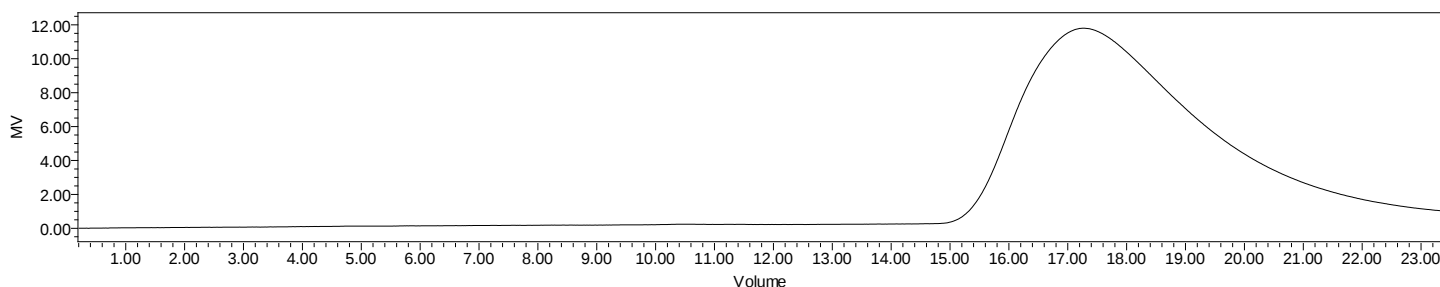

Polymer	M _n (from GPC)	M _w (from GPC)	PDI
P(L)LCL	59,466	77,421	1.30

GPC-ES Analysis Method: Waters Breeze 2 system with 1 ml/min THF flow across three GPC columns. Detection via refractive index, calibrated against polystyrene standards.


DSC

Sample: AP162 250728DJR-A
Size: 3.8000 mg
Method: Modulate-no-epb

DSC

File: C:\...\PolySciTech\AP162 250728DJR-A.001

Run Date: 31-Jul-2025 14:28
Instrument: DSC Q2000 V24.11 Build 124

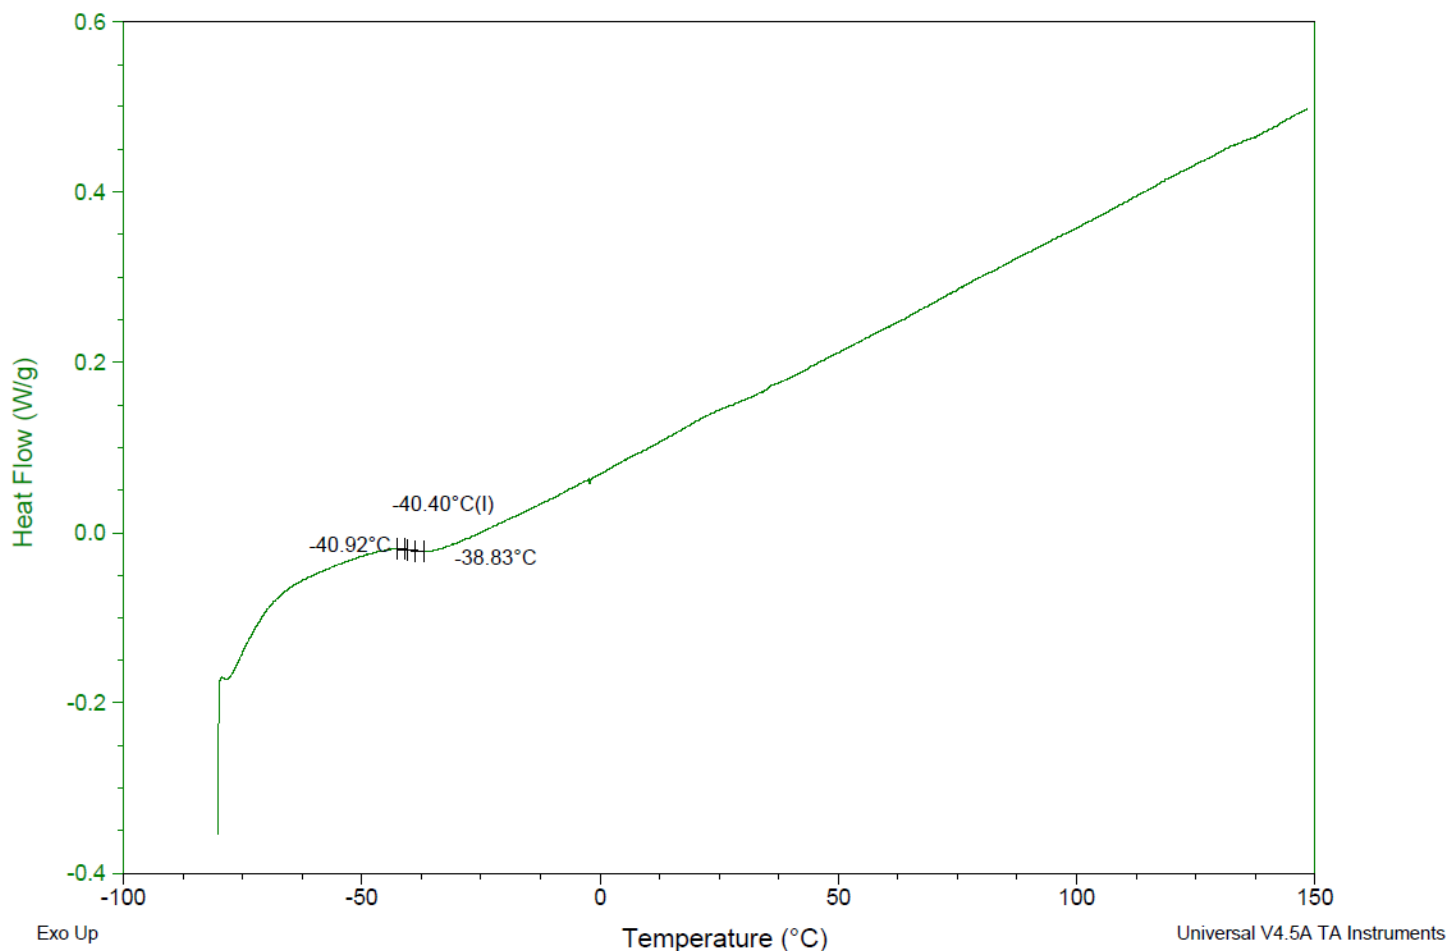


DSC Testing: 1-5 mg sample tested in crimped aluminum pan on a TA Instruments Model Q2000 with procedure equilibraion 100 °C, isothermal 5 minutes, equilibrate -80 °C, data on, ramp 10 °C/min to 150 °C. Tg = -40.4 °C

IV

Inherent Viscosity: 0.371 ± 0.007 dL/g (calculated from kinematic viscosity at 2% w/v Acetone on Rheosense microVISC, n=3) at 25°C.

Structure of copolymers

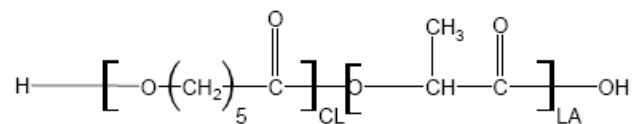

Approved By:
Amie Tyler
Quality Manager