



No. AV005


Certificate of Analysis

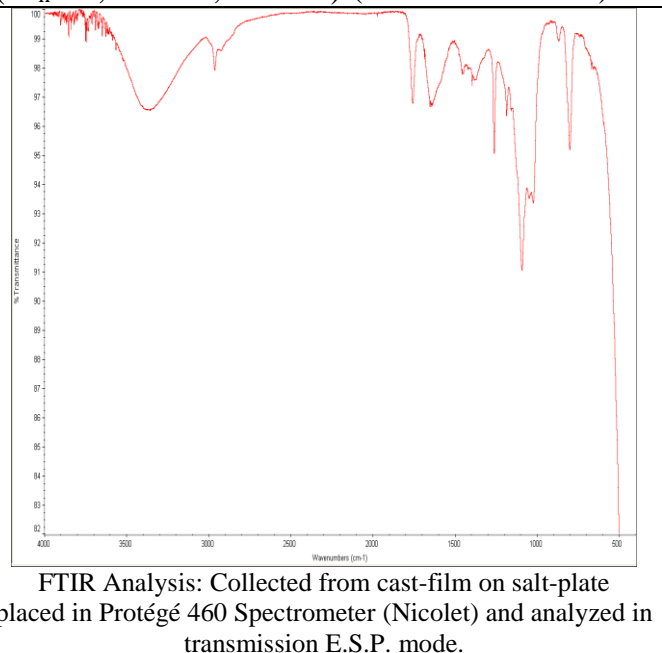

Product Name: Poly(L-lactide)-Fluorescein endcap (M_n 20,000-40,000 Da) (Lot# 70331JSG-A)

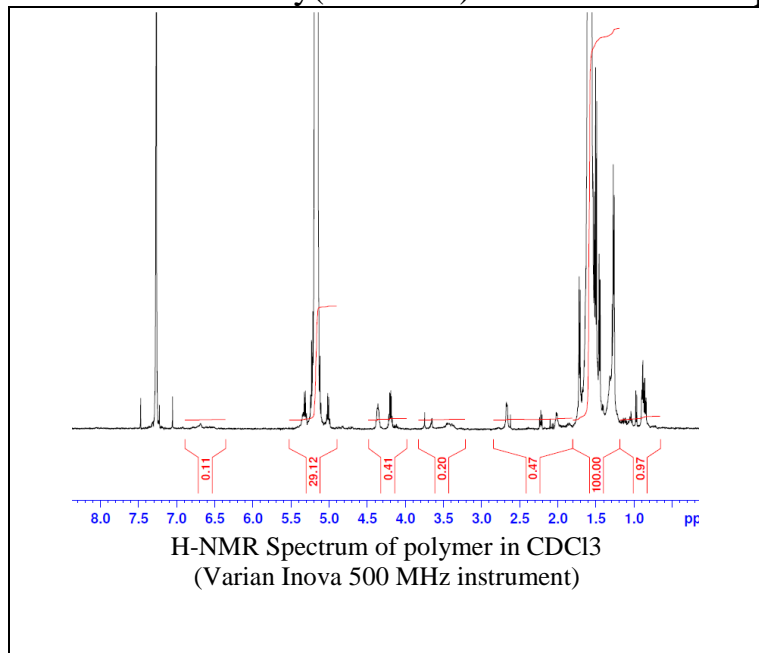

- **GPC analysis of PLLA-Fluorescein polymers**

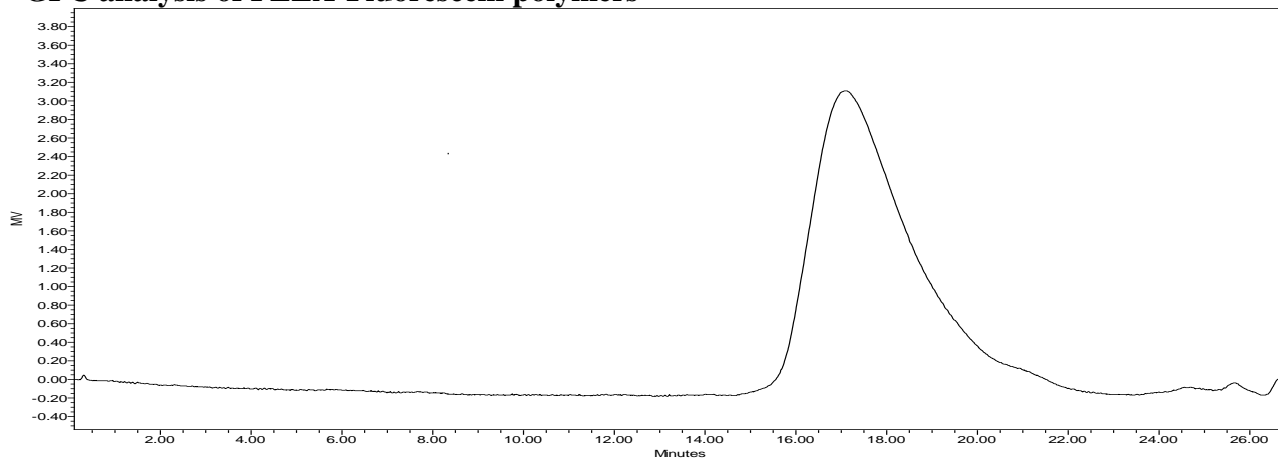

Analysis Method: Waters Breeze 2 system with 1 ml/min THF flow across three GPC columns (mixed porosity). Detection via refractive index, calibrated against polystyrene standards.

Polymer	M_n (from GPC)	M_w (from GPC)	PDI
PLLA-FITC	33,236	46,594	1.40

- **Chemical Structure**

